



COWELL® Implant Solution

Help your daily practice superior
Ver.29




The Beginning of Premium Korean Dental Implant

SINCE
1994

THE OLDEST IMPLANT CASE IN KOREA

1995
START
1994



BioPlant™



Atlas™



INNO Implant™

#35: BIOPLANT™, 1st generation of the COWELL® Implant, Korea's first dental implant developed in 1994.

#25, 36 & 37: ATLAS Implant System™, 2nd generation of the COWELL® Implant, Korea's first ASD treated Implant.

#32, 33 & 47: INNO Implant System®, Cowellmedi's 4th generation implant surface, SLA-SH™ treated implant.


Contents



COWELLMEDI History 004

REID (Research & Education in Implant Dentistry) 006

COWELL® Implant System




- **Introduction**
- Process Flow Chart 008
- COWELL® Warranty 010
- Package System 011
- SLA-SH™ Surface Treatment 016
- COWELL® CLASS 1000 021

- **INNO Implant System®**
- INNO-Fixture Design 024
- Abutment Prosthetic Protocol 026
- INNO Submerged & Short Implant 028
- INNO Submerged Narrow Implant 060
- INNO Internal Implant 076
- INNO External Implant 096
- Surgical Kits 110
- INNO Prosthetic Planning Kit 126
- INNO Prosthetic Instrument Kit 128

- **Mini Plus® Implant System**
- Mini Plus® Implant 129
- Surgical Kit 134


COWELL® Digital Products



- **Digital Guided Surgery Kit**
- InnoFit Lodestar Plus Kit 138
- InnoFit Lodestar Kit 154


- **Digital Prosthesis**
- InnoFit Hybrid Ti-Base System
- Sub. Hybrid Ti-Base System 166
- Sub. & Sub-N. Multi Hybrid Ti-Base System 172
- Sub. Lock Hybrid Ti-Base System 176
- Sub-N. Hybrid Ti-Base System 180
- Int. Hybrid Ti-Base System 184

COWELL® Expert Instruments



- MFS Kit 190
- Easy Sinus Lift Kit 198
- MFR Kit 204
- InnoGenic® GBR Kit 208
- InnoGenic® Autobone Harvester 218
- COWELL® BMP Trephine Kit 223
- Atraumatic Extraction Kit 226
- Direct Surgical Guide Kit 233
- AO4 Surgical Stent 242
- Volume-up™ Guide System 244

COWELL® Regenerative Solution



- COWELL® BMP Series 250
- INNO-CaP 258
- INNO OSS & INNO OSS Allo 260
- DiaBone 261
- MEGA DERM™ Plus 262
- Diaderm® M 264
- InnoGenic® Non-resorbable Membranes 265

COWELLMEDI HISTORY

For the first time in Korea,

Beginning with Korea's First Dental Implant, the COWELLMEDI has been leading the way to the future biomedical industry with the fusion technology to its E.rhBMP-2 developed for the first time in the world.



- 1994** • Developed KOREA'S FIRST DENTAL IMPLANT, BIOPLANT™.
• Succeeded in localizing DENTAL IMPLANT FOR THE FIRST TIME IN KOREA.
- 1998** • Founded Asrahi Medical.
- 1999** • Established R&D corporation with PNU's Oral and Biotechnology Research Center.
- 2000** • Converted to COWELLMEDI corporation (Cowellmedi Co., Ltd.).
• Obtained ISO9001 certificate.
- 2002** • Developed ASD surface treatment technology for dental implant for the first time in Korea.
- 2003** • Obtained US FDA approval for the BIOPLANT™ Implant System.
- 2004** • Medaled for contribution of developing KOREA'S FIRST DENTAL IMPLANT from Korean Government.
- 2005** • Obtained GMP, ISO13485 and CE certificate.
• Obtained US FDA approval for the ATLAS Implant System™.
- 2006** • Established COWELLMEDI USA and COWELLMEDI Taiwan.
• Established COWELLMEDI Tissue Engineering Institute for Growth Factors.
- 2007** • Obtained a KR patent for dental implants coated with E.rhBMP-2, E.Coli derived Recombinant Human Bone Morphogenetic Protein type 2, developed for THE FIRST TIME IN THE WORLD.
- 2008** • Completed preclinical trials on E.rhBMP-2 (COWELL® BMP).
- 2009** • Obtained MFDS approval for clinical trials on the COWELL® BMP.

- 2010** • Obtained MFDS manufacturing and sales approval for the COWELL® BMP.
• Held the 1st WORLD BMP Symposium in Seoul, Korea.
- 2011** • Obtained a US patent for E.rhBMP-2 Coated Implant.
- 2012** • Obtained MFDS Approval for E.rhBMP-2 Spinal Fusion Clinical Test Plan.
• Launched the INNO Implant System®.
- 2013** • Obtained US FDA approval for the the INNO Implant System®.
- 2014** • Established a R&D and Education Organization, REID (Research & Education in Implant Dentistry).
- 2015** • Developed SUPER-HYDROPHILIC implant surface, SLA-SH™.
(Sandblasted, Large-grit, Acid-etched, and Super-Hydrophilised)
- 2016** • Established COWELLMEDI China.
• Established educational cooperation with MMS (Miami Medical Seminars).
- 2017** • Launched the Sonator™ 80's System, an implant-supported overdenture system.
- 2018** • Launched the InnoGenic® Wifi-Mesh, a non-resorbable membrane.
• Appointed as a global IP(Intellectual Property) star enterprise.
- 2019** • Published "20 YEARS OF OUTCOMES, 20 YEARS OF CLINICAL EVIDENCE OF COWELL® Implant System", a clinical case collection with a record of COWELL® Implant System for over 20 years.
- 2020** • Obtained MDSAP certificate.
- 2021** • Obtained CE certificate for the InnoGenic® Wifi-Mesh and PTFE-Mesh.
• Obtained Health Canada approval for the INNO Implant System®.



Research and Education in Implant Dentistry.


The REID is a global institute, standing for Research and Education in Implant Dentistry.

The REID has been dedicated to researching technology and knowledge for implant dentistry, creating more predictable concepts of treatment, and developing cutting-edge products in implant dentistry and related fields as its first objective of the establishment.

As its second objective of the establishment, the REID also has been committed to training dental professionals with world-class clinicians, lecturers, and education curricula.

The REID is now reaching more clinicians with easier access to a variety of clinical solutions and open discussions where everyone can attend.

Should you have any to share with us to achieve our mission together, be a part of us. The REID is always open for you.

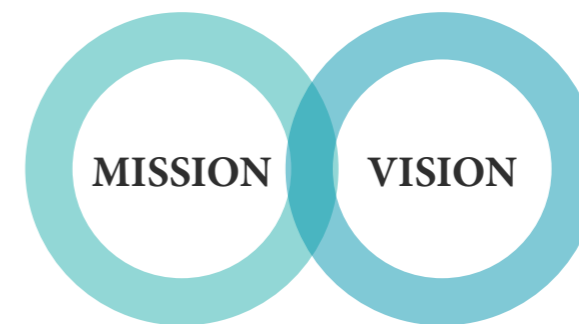


To improve how the world dental community treats implant dentistry by providing dental professionals with internationally multidisciplinary education service and state of the art treatment concepts as well as comprehensive quality research for the benefit of patients.

- Constructing the future of implant dentistry and related fields.
- The world-class education provider and research institute.
- Sharing more know-hows to have better ideas by expanding a worldwide network of members.
- Providing training systems accessible to any dental professional across the globe.

Process Flow Chart

CNC Machining



Precise machining process using state of the art computer numerical control system fused to the COWELL® Class 1000, operated by a world-class technical unit.



Surface Treatment



The SLA-SH™ Surface treatment with biologically active materials to achieve the ideal osseointegration.



Inspection



Absolutely accurate test and quality control system with cutting edge equipment such as optical profiling measurer, stereoscopic microscope, micrometer scope, and other specialized devices for dental implant manufacturing.

Cleansing



The cleansing process by ultrasonic wave using the 3rd distilled water, vacuum dry, and heating dry sterilization leaves no residue and ultimately sterilizes the products.



Packing and Sterilization



Sanitarily packed products at cleanrooms are sterilized by gamma-ray using radiation isotope.



Shipping Warehouse



The finished products are sorted and stored at warehouses for immediate delivery.

COWELL® Warranty

* For more details, visit our website at www.cowellmedi.com

1. Guarantee beneficiary and scope

Products	Period	Conditions	Remarks
Implant	Lifetime	Replacement with equivalent Implant	The period shall begin from the sale date

2. Scope of Warranty

- 1) Quality benefits
> In case the product material or the manufacturing process is flawed.
- 2) Surgical benefits
> In case implants fail to be grafted to the bone.

3. Claim Procedure

- 1) In case certain faults occur after transplanting implants (procedure), the staff in charge shall be contacted within 30 days thereafter.
- 2) When such contact is made, the Customer Complaint Report shall be written out and shall be submitted together with the concerned product.

4. Exclusions from Warranty Service

- 1) In case implants are transplanted onto patients with diabetes and alcohol addiction.
- 2) In case implants are transplanted onto patients for whom surgical procedures are difficult to perform due to the history of the systemic disease.
- 3) In case implants are transplanted onto patients who depend on habitual medications.
- 4) In case the procedure is not conducted according to the protocol of the COWELLMEDI.
- 5) In case the procedure is not performed in compliance with biological indication :
(E.g. distance between the buccal wall and implant should be at least 2mm).
- 6) In case the procedure is conducted using contaminated surgical devices.
- 7) In case implants are transplanted onto patients who sustain or are infected with cell issue contamination.
- 8) In case other materials from other companies are mix-used with Implants, prosthetic parts and instruments of the COWELLMEDI.
- 9) In case the result of investigations by COWELL R&D Institute, Div. of QA and QC shows the issue is not related to the products manufactured and provided by the COWELLMEDI.
- 10) Store at room temperature and in a dry place, and care should be taken from contamination after the product is opened.
- 11) In case the information hereby requested, especially, product Lot no., Serial no. or X-ray photos, is missing.
- 12) In case that the concerned products are not returned.
- 13) In case the product is damaged due to negligence of handling.
- 14) In case the product is opened and fails to remain sterilized.
- 15) In case that the expiry date of the concerned product (not opened products only) is not longer than 1/4.

Package System

1. Color classification (Coding) by fixture type and external label marking

A. Color classification by fixture type

Fixture type	Submerged (Sub.)	Submerged Short (Sub.)	Internal (Int.)	External (Ext.)	Submerged Narrow (Sub-N.)	Mini Cement (1P-C.)	Mini Ball (1P-B.)
Package							
Connection	 Blue	 Orange	 Green	 Emerald	 Pink		

B. External label marking and color coding by fixture diameter & fixture type

- > Color coding by diameter on the external label.
- > Reuse is prohibited after opening as the product is sterilized.
- > After the ampule is opened, care should be taken from dropping, which may be caused by incomplete fastening.
- > Store at room temperature and in a dry place, and care should be taken from contamination after the product is opened.
- > Discard expired products.

20A060040A0004
ST4010SM
Ø4.10mm
INNO Sub. Fixture

INNO Fixture
(No-Mount)

PRODUCT NAME : COWELL® INNO Implant System
CATALOG No. (REF) : ST4010SM
SIZE : Ø4.0X10mm(Sub.Hex.Taper)
LOT NO. (Lot) : 22A060040A
DATE OF MANUFACTURE (M) : 2022-01-06
USE BY : 2027-01-05
PACKING UNIT : 1EA

STORAGE CONDITION : Store at room temperature and in a dry place.

STERILE R Sterilized Using Irradiation

Manufacturer : **Cowellmedi Co., Ltd.**
48, Hakgam-daero 221beon-gil, Sasang-gu, Busan, 46986, Republic of Korea TEL.: +82-51-312-2027~8
Website: <http://www.cowellmedi.com>
D/T : 218 Trianon LN Villanova PA 19085-1442 USA
EC-Representative (EUREP) : Certification Experts B.V.
Amerlandseweg 7, 3621 ZC Breukelen, The Netherlands

(01) 08800016106725
(11) 220106
(10) 22A060040A
(21) 0004

Rx Only
MEDICAL DEVICE CWM-L-004 (Ver.3)

* Ex.) INNO Sub. Fixture (No-Mount)
Dimension: Ø4.0X10mm

Diameter / Fixture Type(abbr.)	Ø2.5	Ø3.0	Ø3.1	Ø3.3	Ø3.5	Ø4.0	Ø4.5	Ø5.0	Ø5.5	Ø6.0
	Bisque	Green	Burgundy	Orange	Yellow	Emerald	Red	Pink	Violet	Gray
Submerged (Sub.)	-	-	-	-	✓	✓	✓	✓	-	✓
Submerged Short (Sub.)	-	-	-	-	-	✓	✓	✓	✓	✓
Internal (Int.)	-	-	-	-	✓	✓	✓	✓	-	✓
External (Ext.)	-	-	-	-	✓	✓	✓	✓	-	✓
Submerged Narrow (Sub-N.)	-	-	✓	✓	-	-	-	-	-	-
Mini Cement (1P-C.)	✓	✓	-	-	-	-	-	-	-	-
Mini Ball (1P-B.)	✓	✓	-	-	-	-	-	-	-	-

2. Fixture user guide (Embedded in the packaging)

COWELL® IMPLANT SYSTEM Instructions for Use

1. Device Description

The COWELLMEDI implant system includes a variety of precision-machined fixtures manufactured from titanium. These implants are surgically inserted into a mandible (the lower jawbone) or a maxillary bone (the upper jawbone) and serve as a replacement for a patient's tooth root providing a stable foundation for restoration.

2. Intended for use

To support dental prosthesis as a dental device, which is implanted into alveolar bone to recover masticatory function and give better esthetics in patients with partially or full edentulous jaws.

3. Directions for use

1) Surgery - The first stage

- According to the patient's condition, appropriate dental cleaning operations may be performed and preventive antibiotics may be administered prior to implant operation.
- Clean and disinfect the operative site, administer local anesthesia in the area and expose the alveolar bone by making appropriate incisions and reflecting the gingival tissues along the alveolar crest in the area from where teeth were extracted.
- Drill into the gum in order to implant a fixture into the planned place with various dental operation tools. The speed of the revolution of the drill should be adjusted by the condition of the bone and the kinds of operation tools. Saline solution should be poured onto the area so that necrosis doesn't occur by heating of the bone (The speed for all drilling should be less than 1,200 rpm).
- Remove the external sterile package cover sheet: open the cap of the ampule: affix the Fixture Driver (in case of No-mount Fixture) or the Mount Driver (in case of Pre-mount Fixture) to the Hand-piece and connect it to the fixture: move the assembled piece to the osteotomy site for the implant using care to prevent the assembled piece from being separated or contaminated with foreign materials.
- A fixture is implanted into the bone as planned depth by turning (25-30 rpm) a hand-piece clockwise with 15-50 N.cm torque. In event that it is hard to insert, extend the width of bone by Tap Drill or Countersink (less than 1,200 rpm) in order to facilitate better implantation.
- After finishing implantation, the treated part should be sutured by using a hex driver to connect to the Cover Screw with torque 5 N.cm to prevent the intrusion of a foreign substance in the fixture.

2) Surgery - The second stage

- Incise gingival of the upper part of fixture subsequent to bone fusion and remove Cover Screw, tighten up Healing Abutment and start gingival curing for a prosthesis.
- In general, surgery is done by a method that makes prosthesis.

4. Contraindication

The operation should be reconsidered when the patient has any of the following conditions.

- Patient with oral infection or inflammation.
- In the case of low-quality bone which will result in an unstable implant.
- Patients who have a drinking problem or mental disease or substance or medicine abuse.
- Internal diseases such as hemato-dyscrasia or diabetes and undernourishment.
- Any patient who is not suitable for operation.

5. Warnings

Implant surgery and restoration involve complex dental procedures. For safe and effective use of the COWELLMEDI fixtures, it is strongly suggested that specialized training be undertaken since the surgical techniques required to place dental implants are highly specialized and complex procedures. Improper patient selection and technique can contribute to fixture failure and/or loss of supporting bone. The COWELLMEDI fixtures are intended for use only in the indicated applications. Dental fixtures must not be altered in any way. The use of electro-surgical instruments or lasers around metallic fixtures and their abutments is not recommended due to the risk of electric shock and/or burns. Fixture mobility, bone loss, or chronic infection may indicate fixture failure. The treatment should be done in an aseptic condition by an operator who wears an aseptic costume. If the fixture becomes contaminated by the patient's body fluids in any way, the fixture cannot be used in any other patient.

6. Precautions

The surgical techniques required to place endosseous dental fixtures require specialized and complex procedures. Formal training for the placement of fixtures is recommended.

Important: Determine local anatomy and suitability of the available bone for fixture placement. Thorough screening of prospective fixture candidates must be performed. Visual inspection as well as panoramic and periapical radiographs are essential to determine anatomical landmarks, occlusal conditions, periodontal

status, and adequacy of bone. Lateral cephalometric radiographs, CT scans and tomograms may also be beneficial. Adequate radiographs, direct palpation and visual inspection of the fixture site are necessary prior to treatment, planning and use of the COWELLMEDI fixtures.

7. Adverse Effects

Some of the complications (loss of fixture anchorage, prosthesis etc.) are possible occurrences after surgery. Lack of quantity or poor quality of remaining bone, infections, poor patient oral hygiene or cooperation, patient discomfort, fixture mobility, local soft tissue degeneration, and unfavorable fixture placement or alignment are some potential causes for loss of anchorage.

8. Surgical complications

The implant procedure has risks, including localized swelling, dehiscence, tenderness of short duration, edema, hematoma or bleeding. Numbness of the lower lip and chin region following lower jaw surgery, and of the tissue beside the nose following upper jaw surgery, is a possible side-effect of the surgery. Though it would most probably be of a temporary nature, in very rare cases, the numbness has been permanent. Gingival mucosal (gum tissue) ulceration, tissue reaction, or infection may occur, but generally responds to local care.

9. Post-implant Management

- The upper jaw requires a healing period of 6-8 months depending on the bone quality, and the lower jaw requires a healing period of 3-5 months, again depending on the bone quality. If pressure is applied to the fixture during the healing period, such as in mastication, early fixation may not be achieved or osseointegration of the fixture may not occur within the healing period.
- Once the operator clinically determines that sufficient osseointegration has been achieved, he/she should begin producing the dental prosthesis.
- The Lot Number Identification Tag and the X-ray film should be attached to the patient's chart, to track the product when needed.
- The operator should determine the osseointegration status of the implant through X-ray and clinical methods such as percussion and/or reverse torquing.

10. Storage / Sterilization and Handling

- Store the product at room temperature and in a dry place.
- The fixture, fixture mount, and cover screw have been cleaned and sterilized through radiation (gamma irradiation) and are ready for use.
- The product packages should be opened just before their use during the operation. Expired products should not be used.
- Only appropriate sterilized surgical tools made specifically for dental implants should be used during the operation.

11. Expiration date

The expiration date of the product is 5 years from manufacturing.

12. Cleaning & Sterilization

Cleaning of surgical instruments supplied non-sterile should be performed according to current dental standard practices. Select a suitable method of cleaning that removes all visible contamination from the product in sterilized and distilled water. After cleaning, package the product appropriately and then sterilized by autoclave at the minimum condition of 250°F (121°C/15 mins).

13. Caution

- As this product is sterilized by Gamma radiation, it should not be used under any circumstances if open.
- Every product is disposable. It should not be reused.

COWELLMEDI Co., Ltd.


48, Hakgam-daero 221beon-gil, Sasang-gu, Busan, 617-801, Republic of Korea
Tel. +82-51-312-2027~8 Fax. +82-51-316-2628
<https://www.cowellmedi.com>

D/T

COWELLMEDI USA INC. 218 Trianon LN Villanova PA 19085-1442 USA
Tel. +1-623-939-1344 Fax. +1-623-939-1472

EC-REPRESENTATIVE

Certification Experts B.V. Amerlandseweg 7, 3621 ZC Breukelen, The Netherlands



2021. 09. 02 / CWM-I-007 (Ver.4)

3. Fixture packaging opening and the sequence of the product extraction



Taking out the ampule




- 1 Press the upper dotted area to open, and take out the sterilized blister pack.



- 2 Remove the moisture-resistant paper on the back of the blister pack, and drop the ampule lightly on the palm of a practitioner or surgical clothes.

Fixture separation




- 1 Hold the ampule with both hands and twist it 45 degrees to separate the middle part. Care should be taken to prevent the fixture from falling off.




- 2 Fixtures are fastened in two ways.
 - 1) No-Mount -> Fasten with the Fixture Driver.
 - 2) Pre-Mount -> Fasten with the Mount Driver.

Cover Screw separation



- 1 Separate the upper part of the ampule.




- 2 Fasten the Hex Driver to the Cover Screw completely. Care must be taken to prevent the patient from swallowing the Cover Screw at the time of placing.

4. Abutment packaging and external label marking



5. Surgical Kit packaging and external label marking



Implant Innovation
 When INNOVATION meets Dental Implant.

Achieving cell-to-cell communication with SLA-SH™

made with the longest experience in Korea

Superhydrophilicity, Uniform micro-surface geometry, Maximized BIC, and Acceleration of osseointegration

Aspiring for 100% perfection with SLA-SH™



SLA-SH™ Surface Treatment

Achieving cell-to-cell communication


SLA-SH™:

Sandblasted, Large-grit, Acid-etched, and Super-Hydrophilised


- > Long-lasting super-hydrophilic activation by special soaking technology.
- > Al₂O₃ free, sandblasted with biocompatible grits unlike the majority of other implants sold in the market.
- > Macro-pore & micro-pore of Ti-oxide layer mimicking the etched enamel rod of the tooth.
- > Even distribution of roughness through the whole portion of the implant surface.
- > No destruction or alteration of the surface is caused even with torque force of 120 N.cm.
- > Acceleration of osseointegration and maximization of BIC.

1. Evaluation using SEM (Scanning Electron Microscope) Images

A. SLA-SH™ Surface magnified X300, 1,000 and 3,000




B. Comparison to other SLA treated implants currently sold in the market




- > Surface treatment patterns were observed on electron microscope photographs of 5,000 magnifications for top parts of the implants.
- > Sand-blasted surface conditions were observed in the product A, B, and C due to insufficient acid etching patterns in deep parts as the SLA-SH™ is sandblasted with biocompatible grits with even particle size unlike others are done with alumina.
- > The entire surface of the SLA-SH™ treated implant showed uniform acid etching patterns. This implies that the acid etching of the SLA-SH™ surface is perfect.

2. Evaluation using SSEM (Stereo Scanning Electron Microscope) 3D images

A. SLA-SH™ Surface

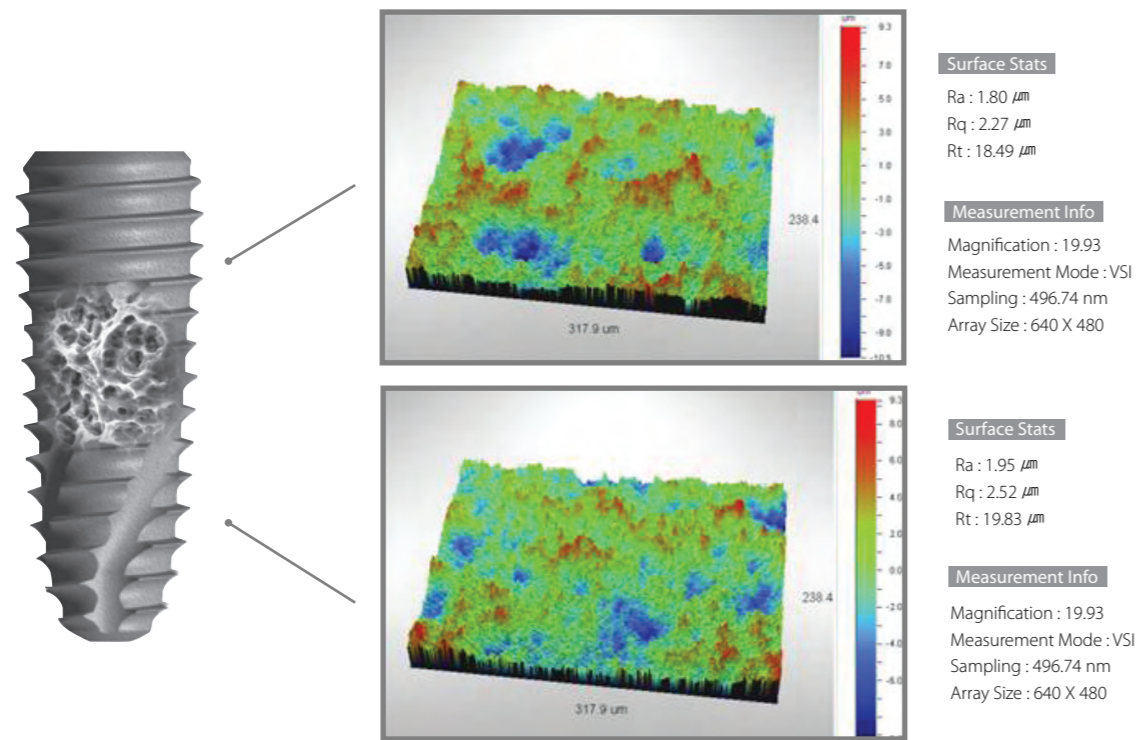


B. Comparison to other SLA treated implants currently sold in the market

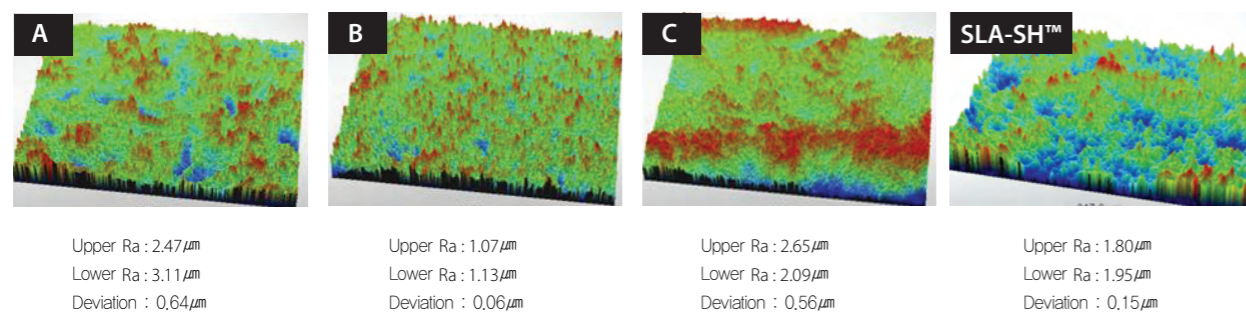

- > Uniform distribution of Macro-pore and micro-pore.
- > Roughness of the SLA-SH™ showed 1.90 μm while the others were 1.08 to 3.11 μm .

3. The surface activity increased due to the great surface wetness

A. Contact angle measurement evaluation result for the saline solution




After the hydrophilic and super-hydrophilic activation by special soaking technology, the sample became extremely hydrophilic and the surface energy increased, which facilitated the expedition of osteoblast activation to fuse to the bone faster.

Capillarity in the actual clinical setting, which accelerated the penetration of blood.
※ Quoted from the website of Cowellmedi Clinical Research Group (www.e-cowellmedi.com)



B. Relation between surface wetness and roughness



> There was almost no difference in surface roughness and micro-geometry, and the difference of surface wetness took place in the same physicochemical properties as surface energy increased by hydrophilic activation treatment.

C. Physicochemical alteration of surface by hydrophilic activation treatment

Name	Start BE	Peak BE	End BE
C1s	290	284.6	280.5
O1s	535.3	530.42	525.6
Ti2p	468.1	458.78	450.4

After SLA treatment


Name	Start BE	Peak BE	End BE
C1s	290.46	284.6	284.6
O1s	538.8	533.73	529.3
Ti2p	468.2	456.76	453.4

After hydrophilicity activation treatment

- > Surface wetness was improved by the increased surface energy of C1s, O1s and Ti2p after hydrophilic activation treatment.
- > To maintain and even to enhance surface wetness, super-hydrophilic activation treatment was carried out and contamination by carbon in the atmosphere is prevented during packing and sterilization.

4. Its safety has been proven through perfect cleaning with an automated system

A. Comparison of surface element tests through X-ray diffraction



> Cutting-edge automated system that produces the 3rd distilled water.

B. Comparison of surface element tests (X-ray Photo-electron Spectroscopy, XPS)

Sample	Unit : %				
	C1s	O1s	Ti2p	Si2p	N1s
A	34.12	45.05	15.11	5.24	0.47
B	31.84	46.49	15.22	4.87	1.57
C	32.19	47.58	17.58	2.65	N.D
SLA-SH™	27.19	50.81	17.61	N.D	N.D

> Quantitative analysis of each surface element found 30% carbon, 47% oxygen, 16% titanium, and 4% silicon in all products.

> For the SLA-SH™, they only consisted of carbons(C1s), oxygen(O1s), and titanium(Ti2p).

> Sodium hydroxide, the main element of the alkali washing solution, combined with silicon(Si) to form water-soluble $\text{Na}_2\text{SiO}_2(\text{OH})_2 \cdot 4\text{H}_2\text{O}$ (water glass), which removed the other elements.

C. Comparison of elution tests using combustion ion chromatography

Sample	Unit : ppm						
	F ⁻	Cl ⁻	NO ₂ ⁻	SO ₄ ²⁻	Br ⁻	NO ₃ ⁻	PO ₄ ³⁻
A	N.D	0.024	0.027	0.002	N.D	0.031	N.D
B	N.D	0.027	0.019	0.002	N.D	0.030	N.D
C	N.D	0.071	0.020	N.D	N.D	0.023	N.D
SLA-SH™	N.D	N.D	N.D	N.D	N.D	0.032	N.D

> Similar ions were detected in all the products, but they are not harmful to humans because their elements and quantities do not affect the human body and those have been proven in many studies.


> For the SLA-SH™, no other elements except for NO₃⁻ were detected. Alkali washing completely removed the SO₄²⁻ and Cl⁻ ions of sulfuric acid and hydrochloric acid, which are used for heated acid etching because they form water-soluble salts of Na₂SO₄ and NaCl.

> No elements that interfere with osteo anagenesis were found from both the surface and elution elements, which shows that the cleansing process was perfectly carried out.

COWELL® CLASS 1000


A SUBTLE DIFFERENCE MAKES THE DENTAL IMPLANT OR NOT

1. Fixture manufacturing tolerance evaluation



Evaluation Item	Manufacturing Tolerance				
Method	a. The specimen was fixed in Jig. b. Each dimensional difference of 3 inner hexagonal connection sides (Hex-1, Hex-2, Hex-3) of 5 specimens was measured.				
Used Equipment	Measuring Microscope and Jig				
Criteria	Each dimensional difference of 3 inner hexagonal sides is no more than ±0.001mm (1.000μm) from 2.500mm.				
Specimen	INNO Submerged Fixture (5 Pieces of ST4510S)				
	#1	#2	#3	#4	#5
Hex-1	2.499	2.500	2.500	2.500	2.500
Hex-2	2.500	2.500	2.501	2.500	2.500
Hex-3	2.500	2.500	2.500	2.501	2.499
Average	2.500	2.500	2.500	2.500	2.500
Total Average	2.500				
Result (Pass/Fail)	Pass				
Manufacturing Tolerance	No more than ±0.001mm (1.000μm)				

2. Prosthetic component manufacturing tolerance evaluation



Evaluation Item	Manufacturing Tolerance				
Method	a. The specimen was fixed in Micro-Measuring Instrument. b. Each dimensional difference of 3 outer hexagonal connection sides (Hex-1, Hex-2, Hex-3) of 5 specimens was measured.				
Used Equipment	Micro-Measuring Instrument				
Criteria	Each dimensional difference of 3 outer hexagonal connection sides is no more than ±0.001mm (1.000μm) from 2.490mm.				
Specimen	INNO Sub. Cemented Abutment (5 Pieces of 2SCH4515)				
	#1	#2	#3	#4	#5
Hex-1	2.489	2.490	2.490	2.490	2.490
Hex-2	2.490	2.490	2.490	2.490	2.490
Hex-3	2.490	2.490	2.490	2.490	2.491
Average	2.490	2.490	2.490	2.490	2.490
Total Average	2.490				
Result (Pass/Fail)	Pass				
Manufacturing Tolerance	No more than ±0.001mm (1.000μm)				

COWELL® IMPLANT SYSTEM

Help your daily practice superior

COWELL®
IMPLANT
SYSTEM


INNO Submerged Narrow Fixture

Designed for the anterior esthetic zone with the narrow alveolar ridge. Double tapered threads acquire higher primary stability through a wedge action.




INNO Submerged Short Fixture

Designed for severe bone resorption. Wide and deep upper threads prevent the compressive necrosis of the cortical bone.



Miniplus® Fixture

Designed for mandible anterior spaces and edentulous arch. Semi-permanent or temporary solution for anterior spaces with the extremely narrow ridge.



INNO External Fixture

The platform neck with open thread aids in the stable engraftment of the periosteum at the bone-implant interface.



INNO Submerged Fixture

Designed for all clinical cases, including immediate implant placement, immediate loading, implant depth adjustment, maxillary sinus, etc. Simply doing all for your implant treatment.

INNO Internal Fixture

4 spiral round cutting edges maximize the efficiency of self-tapping with a sharp edge and accommodate bone chips as ideal cutting edge pocket space.



Volume-up™ Healing Abutment

Devised to prevent food penetration and form aesthetic cervical areas by restoring the contracted buccal alveolar bone and gingiva to their original shape and width.



Meta G UCLA Abutment

Castable abutment with a metal base that can be modified into angulated, telescopic, and custom abutment.




Easy Temporary Abutment

Temporary restoration for the anterior esthetic zone that offers a simpler, speedier, and safer chair-side process.




Angulated Abutment

A simple solution for the anterior esthetic zone.



Milling Abutment

Block abutment to customize contouring.



Multi S&A Abutment

Designed for both edentulous and partially edentulous arches. A broad range of prosthetic options meets diverse clinical requirements.




Lock Abutment

Designed for the same purpose as the Multi S&A Abutment, but for prosthetic restorations in narrow ridges.



Cemented Abutment

The anti-rotational face prevents the prosthesis from rotating, keeping the prosthesis stable.



Sonator 80's S&A Abutment

Designed for use with removable implant-supported overdentures in whole or part by endosseous implants in maxilla and mandible.



Beauty-up™ Abutment

Specially designed to solve esthetical and functional challenges when SCRIP with angulated screw channel is required in the anterior portion.




Ball Abutment

Used to treat patients with minimal standards of care for implant-supported overdentures at an affordable cost.



INNO-Fixture Design



Tapered Hex Connection with Double Contacts


- > Allows for an ideal cold welding between the fixture and abutment.
- > Prevents micro-sinking of the abutment.
- > Minimizes micromovement and distribute stress against loading.

Wide and Deep Upper Threads


- > Prevent the compressive necrosis of the cortical bone.
- > Minimize the need for countersink drills.
- > Increase the mechanical strength by reinforcing the thickness.

Double Tapered Threads

- > Ensure initial stability even in areas with poor bone quality or alveolar socket.
- > Allow the fixture inserted more than half its length into the drilled hole to be placed in only 2 to 4 turns.
- > Achieve higher primary stability with wedge action, even with an additional half turn.



Shortens the placement time with 5mm or more of already entered depth as well as double thread.



Platform Neck

- > Enables stable engraftment of the periosteum at the interface between bone and implant.

Open Threads

- > Allow the fixture to be placed deeper without additional drilling.

4 spiral round cutting edges

- > Maximize the efficiency of self-tapping with sharp edges.
- > Allow for smooth placement of the fixture but provide higher initial stability (see test table below).

Concave Apex Threads with Sharp Cutting Edges

- > Prevent Schneiderian membrane from being ripped.
- > Enhance initial stability of the fixture in extraction sockets.

* Comparison of the average placement torque force of 4 different fixtures (4pcs each) with dimensions of Ø4.5X10mm in 5.0 and 5.5mm deep holes of type 2 bone quality test block.

Classification	INNO	A	B	C
Depth 5.0mm	26.2 N.cm	29.2 N.cm	26.8 N.cm	28.4 N.cm
Depth 5.5mm	44.0 N.cm	38.0 N.cm	34.4 N.cm	38.5 N.cm

Advantageous design for all clinical cases such as immediate implant placement and loading, implant placement & immediate loading, implant depth adjustment, maxillary sinus, and etc.

Fixture type	Submerged (Sub.)	Submerged Short (Sub.)	Internal (Int.)	External (Ext.)	Submerged Narrow (Sub-N)
Fixture Design					
Connection	SUB. HEXAGON SYSTEM		INT. OCTAGON SYSTEM	EXT. HEXAGON SYSTEM	SUB-N. HEXAGON SYSTEM

Simpler, Speedier, and Safer Surgical Kits

Providing dedicated kits for different types of fixtures.



All in One Drill: Minimal drilling frequency with Initial and Final Drill

Chair time for implantation is shortened because the fixture can be implanted with just three times of drilling for general bone quality (Fixture Ø3.5 to 4.5).



Abutment Prosthetic Protocol

> For digital procedure, refer to the COWELL® Digital Products (Refer to the page 166 to 187).

1. Fixture Level Impression - Prosthesis Fabrication

* Two Piece Screw Retained Abutment

Submerged & Submerged Short : Temporary | Easy Temporary

External : Temporary


* Two Piece Screw-Cement Retained / Cement Retained Abutment

Submerged & Submerged Short : Cemented | Angulated | Beauty-up™ | Milling | Meta G UCLA | Plastic UCLA
Hybrid S | Hybrid L | Hybrid A | Ti-Block

Submerged Narrow : Cemented | Angulated | Temporary | Meta G UCLA | Hybrid S | Hybrid L | Hybrid A

Internal : Cemented | Angulated | Meta G UCLA | Hybrid S | Hybrid L

External : Cemented | Angulated | Temporary | Meta G UCLA | Plastic Sleeve

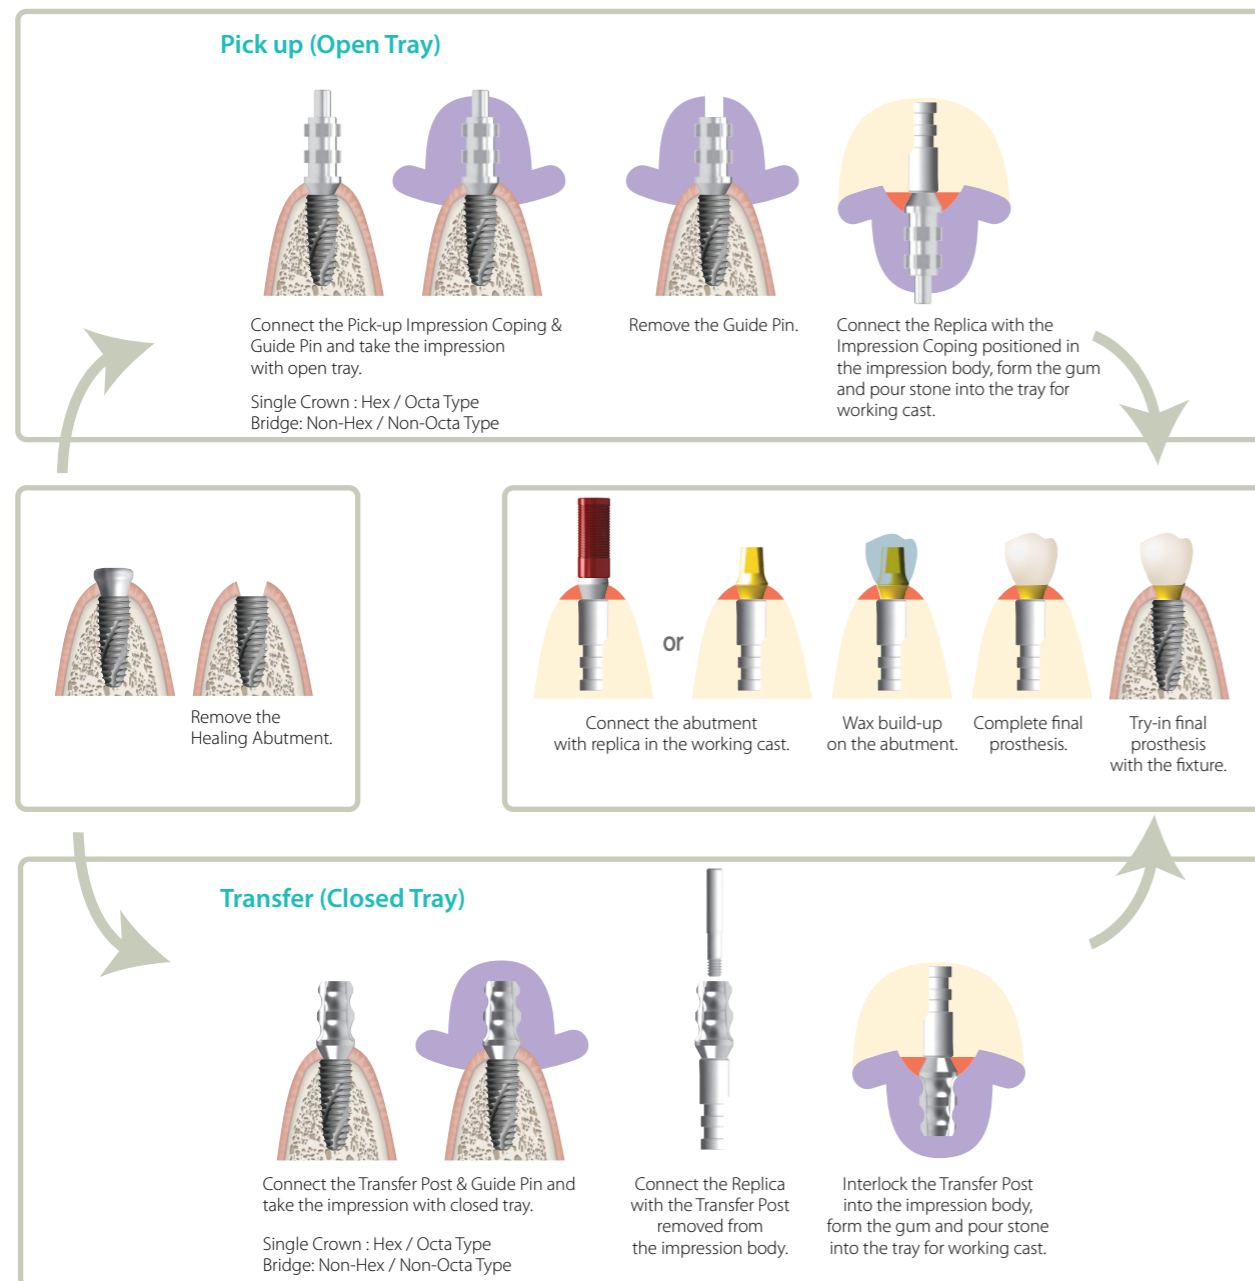

2. Abutment Level Impression - Prosthesis Fabrication

* Two / One Piece Screw Retained Abutment

Submerged & Submerged Short : Multi S | Multi A | Lock

Submerged Narrow : Multi S | Multi A

* One Piece Cemented Retained Abutment

Submerged & Submerged Short : Absolute | Straight (Direct)

Submerged Narrow : Straight

Internal : Solid | Shoulder

External : Shoulder


* Two / One Piece Attachment Retained Abutment

Submerged & Submerged Short : Sonator S | Sonator A | Ball


Internal : Sonator S | Ball

External : Ball

Indirect Impression Technique (No Abutment Modification Applied)

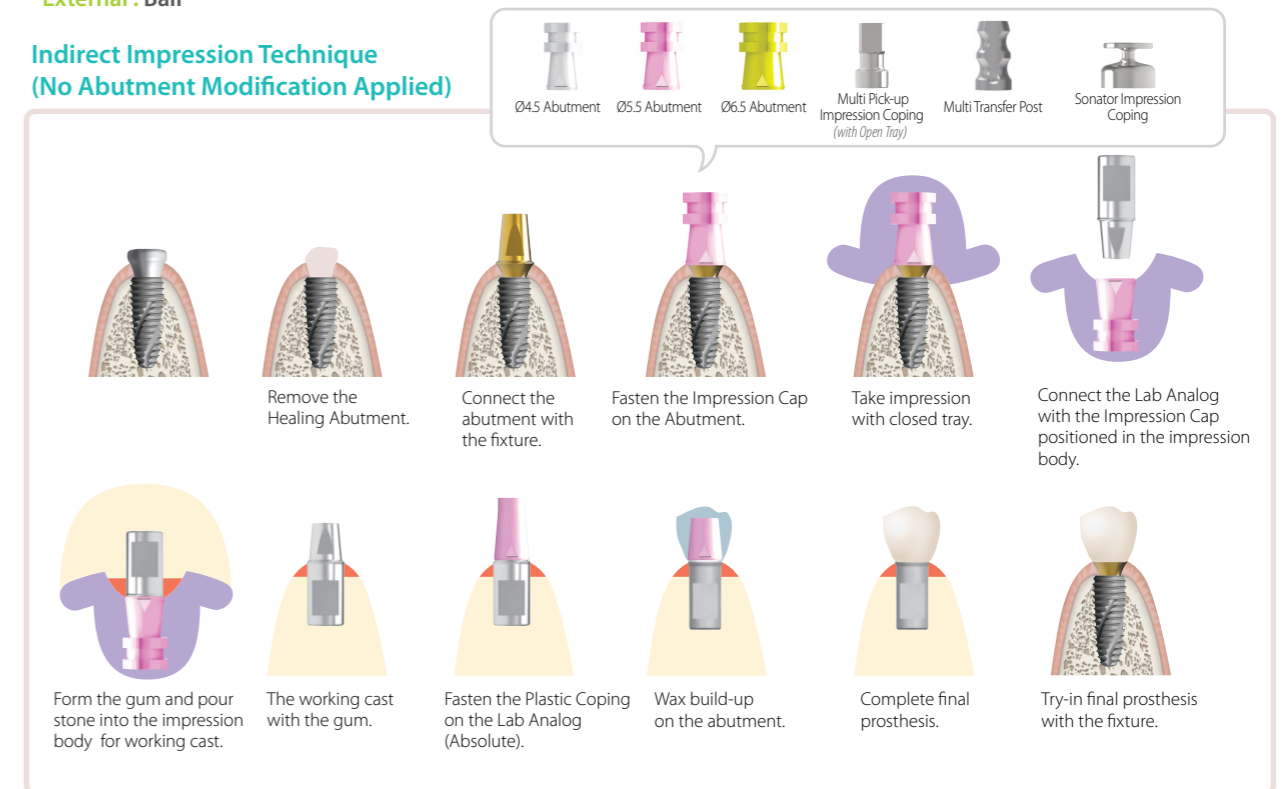

Direct Impression Technique (Abutment Modification Applied)

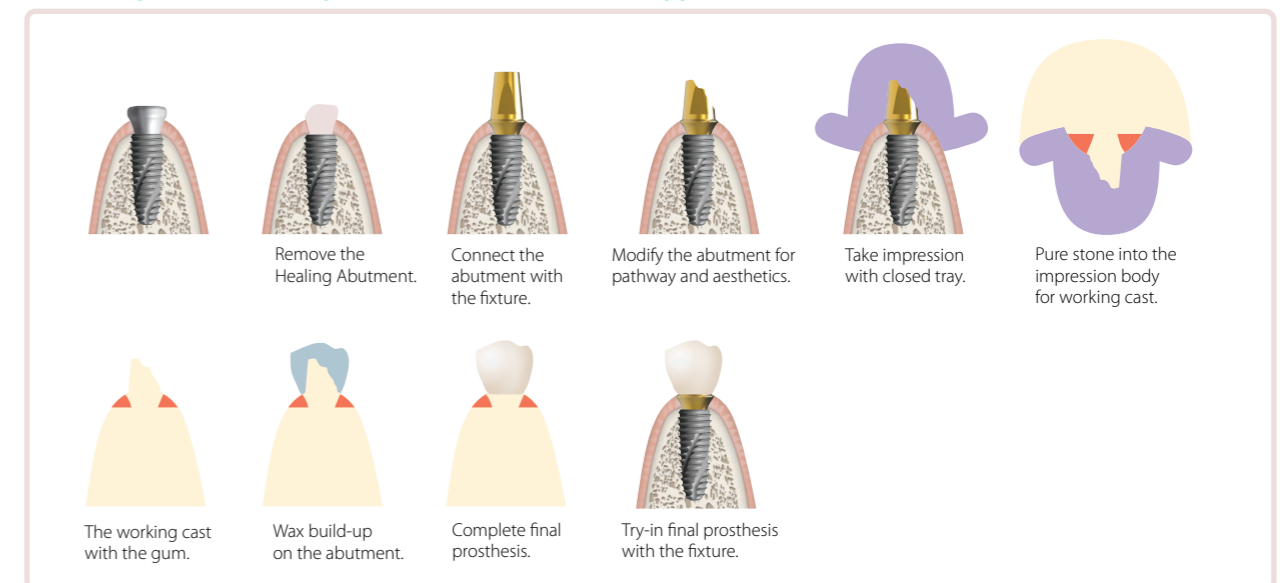


INNO SUBMERGED IMPLANT (Sub.)

System Flow


Fixture	Abutment	Impression
	Prosthetic Procedure I 036p Cemented Abutment, 036p Angulated Abutment, 037p Beauty-up™ Abutment, 037p Milling Abutment, 037p Easy Temporary Abutment, 038p Temporary Abutment, 038p Meta G UCLA Abutment, 038p Plastic UCLA Abutment	Fixture Level Impression 039p Replica, 040p Bite Impression Coping, 040p Pick-up Impression Coping, 040p Transfer Post
	Prosthetic Procedure II 042p Multi S Abutment, 042p Multi A Abutment, 044p Multi Meta G ULCA Cylinder, 044p Multi Plastic UCLA Cylinder, 045p Multi Titanium Cylinder	043p Multi Protection Cap, 043p Multi Pick-up Impression Coping, 043p Multi Transfer Post, 044p Multi Lab Analog
	Prosthetic Procedure III 048p Lock Abutment, 049p Lock Meta G UCLA Cylinder, 049p Lock Titanium Cylinder	048p Lock Protection Cap, 048p Lock Pick-up Impression Coping, 049p Lock Lab Analog
	Prosthetic Procedure IV 052p Absolute Abutment	052p Absolute Protection Cap, 052p Absolute Impression Cap, 052p Absolute Lab Analog, 052p Absolute Plastic Coping
	Prosthetic Procedure V 053p Straight Abutment	Direct Impression
	Prosthetic Procedure VI 055p Sonator S Abutment, 055p Sonator A Abutment	056p Sonator Impression Coping, 057p Sonator Analog
	Prosthetic Procedure VII 059p Ball Abutment	059p Ball Analog

INNO Submerged Implant




Submerged Fixture
Surface Treatment: **SLA-SH™**

- > Interchangeable with hexagonal morse tapered fixture.
- > Internal hex connection (Taper 11°/ Hex 2.5).




No-Mount > Packing unit: 1 Fixture + 1 Cover Screw.


Diameter	Length	Part Number
Ø3.5	7	-
	8	ST3508SM
	10	ST3510SM
	12	ST3512SM
	14	ST3514SM




Diameter	Length	Part Number
Ø4.0	7	ST4007SM
	8	ST4008SM
	10	ST4010SM
	12	ST4012SM
	14	ST4014SM
	16	ST4016SM
	18	ST4018SM




Diameter	Length	Part Number
Ø4.5	7	ST4507SM
	8	ST4508SM
	10	ST4510SM
	12	ST4512SM
	14	ST4514SM
	16	ST4516SM
	18	ST4518SM



Diameter	Length	Part Number
Ø5.0	7	ST5007SM
	8	ST5008SM
	10	ST5010SM
	12	ST5012SM
	14	ST5014SM



Diameter	Length	Part Number
Ø6.0	7	ST6007SM
	8	ST6008SM
	10	ST6010SM
	12	ST6012SM
	14	-



INNO Fixture Code

S Type Submerged | **T** body Taper | **40** Diameter Ø4.0 | **10** Length 10mm | **S** Surface Treatment SLA | **M** Mount No-Mount


* Ex.) SLA No-Mount **ST4010SM**

S Type Submerged | **T** body Taper | **40** Diameter Ø4.0 | **10** Length 10mm | **S** Surface Treatment SLA | **□** Mount Pre-Mount


* Ex.) SLA Pre-Mount **ST4010S**

Pre-Mount > Packing unit: 1 Fixture + 1 Cover Screw + 1 Mount.


Diameter	Ø3.5
Length	
7	-
8	ST3508S
10	ST3510S
12	ST3512S
14	ST3514S




Diameter	Ø4.0
Length	
7	ST4007S
8	ST4008S
10	ST4010S
12	ST4012S
14	ST4014S
16	ST4016S
18	ST4018S




Diameter	Ø4.5
Length	
7	ST4507S
8	ST4508S
10	ST4510S
12	ST4512S
14	ST4514S
16	ST4516S
18	ST4518S



Diameter	Ø5.0
Length	
7	ST5007S
8	ST5008S
10	ST5010S
12	ST5012S
14	ST5014S



Diameter	Ø6.0
Length	
7	ST6007S
8	ST6008S
10	ST6010S
12	ST6012S
14	-




INNO Submerged Short Implant




Submerged Short Fixture
Surface Treatment: **SLA-SH™**

- > Interchangeable with Hexagonal Morse Tapered Fixture.
- > Internal hex connection (Taper 11°/ Hex 2.5).




Pre-Mount > Packing Unit: 1 Fixture + 1 Cover Screw + 1 Mount.


Diameter	Ø4.0
Length	
4	2ST4004S




Diameter	Ø5.5
Length	
4	2ST5504S




Diameter	Ø4.5
Length	
4	2ST4504S




Diameter	Ø6.0
Length	
4	2ST6004S



Diameter	Ø5.0
Length	
4	2ST5004S



Fixture Mount



Length	5.4
	2SMHR001

- > Packing unit: 1 Mount + 1 Mount Screw.
- > Tightened with the 1.2 Hex Driver.
- > Tightening torque force: 5~10N.cm.


Cover Screw



Diameter	Ø3.35	Ø3.75	Ø4.15
Length	3	4.2	5.2
	2SCS000	* 2SCS001	* 2SCS002

- > Packing unit: 1 Cover Screw. *Extra Product
- > To seal the conical interface of the fixture.
- > The longer Cover Screw for the deeply inserted fixture.
- > Tightened with the 1.2 Hex Driver.
- > Tightening torque force: 5~10N.cm.


Healing Abutment



Diameter	Ø4.5		Ø5.5		Ø6.5	
Length	1	2	1	2	1	2
Cuff	2HS4511		2HS5511		2HS6511	
	2	2HS4522	2HS5522	2HS6522		
	3	2HS4532	2HS5532	2HS6532		
	4	2HS4542	2HS5542	2HS6542		
	5	2HS4552	2HS5552	2HS6552		
	7	2HS4572	2HS5572	2HS6572		
Diameter	Ø7.5		Ø8.5		Ø9.5	
Length	2		2		2	
Cuff	2HS7532		2HS8532		2HS9532	


- > Packing unit: 1 Healing Abutment.
- > For remodeling gingival contour during soft tissue healing.
- > Select the abutment according to gingival height and abutment type.
- > Tightened with the 1.2 Hex Driver.
- > Tightening torque force: 5~10N.cm.

Volume-up™ Healing Abutment




Diameter	Ø6.5	Ø7.5	Ø8.5
Length	2	2	2
Cuff	3	VUHN7532	VUHN8532

- > Packing unit: 1 Volume-up™ Healing Abutment (Inbuilt Abutment Screw).
- > Used for an implant procedure to form the gingival tissue and alveolar bone in the form of natural teeth and gums by prevention or minimizing the food penetration.
- > Extremely effective when used with the COWELL® BMP.
- > Recommended to use with the Volume-up™ Guide System.
- > Select the abutment according to gingival height and abutment type.
- > Tightened with the 1.2 Hex Driver.
- > Tightening torque force: 25~35N.cm.




Prosthetic Procedure I

Components Selection Guide for Cemented and UCLA Abutment



Cemented Abutment




Type	Hex								
Diameter	Ø4.5			Ø5.5			Ø6.5		
Length Cuff	4	5.5	7	4	5.5	7	4	5.5	7
1	2SCH4514	2SCH4515	2SCH4517	2SCH5514	2SCH5515	2SCH5517	2SCH6514	2SCH6515	2SCH6517
2	2SCH4524	2SCH4525	2SCH4527	2SCH5524	2SCH5525	2SCH5527	2SCH6524	2SCH6525	2SCH6527
3	2SCH4534	2SCH4535	2SCH4537	2SCH5534	2SCH5535	2SCH5537	2SCH6534	2SCH6535	2SCH6537
4	2SCH4544	2SCH4545	2SCH4547	2SCH5544	2SCH5545	2SCH5547	2SCH6544	2SCH6545	2SCH6547
5	2SCH4554	2SCH4555	2SCH4557	2SCH5554	2SCH5555	2SCH5557	2SCH6554	2SCH6555	2SCH6557

Type	N-Hex								
Diameter	Ø4.5			Ø5.5			Ø6.5		
Length Cuff	4	5.5	7	4	5.5	7	4	5.5	7
1	2SCN4514	2SCN4515	2SCN4517	2SCN5514	2SCN5515	2SCN5517	2SCN6514	2SCN6515	2SCN6517
2	2SCN4524	2SCN4525	2SCN4527	2SCN5524	2SCN5525	2SCN5527	2SCN6524	2SCN6525	2SCN6527
3	2SCN4534	2SCN4535	2SCN4537	2SCN5534	2SCN5535	2SCN5537	2SCN6534	2SCN6535	2SCN6537
4	2SCN4544	2SCN4545	2SCN4547	2SCN5544	2SCN5545	2SCN5547	2SCN6544	2SCN6545	2SCN6547
5	2SCN4554	2SCN4555	2SCN4557	2SCN5554	2SCN5555	2SCN5557	2SCN6554	2SCN6555	2SCN6557

- > Packing unit: 1 Cemented Abutment + 1 Abutment Screw.
- > For Screw-Cement or Cement Retained Prosthesis.
- > Cutting surface for anti-rotation of the prosthesis.
- > Gold color for more translucent restoration.
- > Library available for EXOCAD®, 3Shape® & Others.
- > Connected with the Abutment Screw (2SSHR200).
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 30N.cm.
- > Use the Scanbody for 3D Work.
- > Fixture level impression.

Angulated Abutment




Type	Hex-A				Hex-B			
Diameter(Angle)	Ø4.5(15°)	Ø4.5(25°)	Ø5.5(15°)	Ø5.5(25°)	Ø4.5(15°)	Ø4.5(25°)	Ø5.5(15°)	Ø5.5(25°)
Length Cuff	8	8	8	8	8	8	8	8
1	2SAH45151	2SAH45251	2SAH55151	2SAH55251	2SAH45151B	2SAH45251B	2SAH55151B	2SAH55251B
2	2SAH45152	2SAH45252	2SAH55152	2SAH55252	2SAH45152B	2SAH45252B	2SAH55152B	2SAH55252B
3	2SAH45153	2SAH45253	2SAH55153	2SAH55253	2SAH45153B	2SAH45253B	2SAH55153B	2SAH55253B
4	2SAH45154	2SAH45254	2SAH55154	2SAH55254	2SAH45154B	2SAH45254B	2SAH55154B	2SAH55254B

Type	N-Hex			
Diameter(Angle)	Ø4.5(15°)	Ø4.5(25°)	Ø5.5(15°)	Ø5.5(25°)
Length Cuff	8	8	8	8
1	2SAN45151	2SAN45251	2SAN55151	2SAN55251
2	2SAN45152	2SAN45252	2SAN55152	2SAN55252
3	2SAN45153	2SAN45253	2SAN55153	2SAN55253
4	2SAN45154	2SAN45254	2SAN55154	2SAN55254

- > Packing unit: 1 Angulated Abutment + 1 Abutment Screw.
- > For Screw-Cement or Cement Retained Prosthesis.
- > Solution for the anterior esthetic zone.
- > Connected with the Abutment Screw (2SSHR100).
- > Gold color for more translucent restoration.
- > Select Hex-A or Hex-B according to the case.
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 30N.cm.
- > Fixture level impression.

Beauty-up™ Abutment



Type	Hex	N-Hex	Hex	N-Hex
Diameter(Angle)	Ø3.8 (15°)	Ø3.8 (15°)	Ø3.8 (25°)	Ø3.8 (25°)
Length Cuff	5	5	5	5
2	2SBH381525	2SBN381525	2SBH382525	2SBN382525


- > Packing unit: 1 Beauty-up™ Abutment (Inbuilt Abutment Screw).
- > For Screw-Cement Retained Prosthesis with angulated screw channel.
- > The ultimate solution for the anterior esthetic zone.
- > The gingival line of the Beauty-up™ Abutment allows more esthetic prosthesis.
- > Oval design allows lower incisal application (Mesiodistal diameter: 3.8mm).
- > Tightened with the Angulated Screw Ratchet Driver and Torque Wrench.
- > Tightening torque force: 30N.cm.
- > Library available for EXOCAD®, 3Shape® & Others.
- > Use the Scanbody for 3D Work.
- > Fixture level impression.

* Angulated Screw Ratchet Driver

Height	Type	Ratchet
24(Short)		KRBUD15
29(Long)		KRBUD20

- > Stable to internal slip or fracture due to wide contact area of the Angulated Driver and the dedicated Stargrip Abutment Screw.
- > Tightening torque force: 30N.cm (50N.cm Max.).


Milling Abutment



Type	Hex			N-Hex		
Diameter	Ø4.5	Ø5.5	Ø6.5	Ø4.5	Ø5.5	Ø6.5
Length Cuff	7	7	7	7	7	7
2	2SMH4527	2SMH5527	2SMH6527	2SMN4527	2SMN5527	2SMN6527
4	2SMH4547	2SMH5547	2SMH6547	2SMN4547	2SMN5547	2SMN6547

- > Packing unit: 1 Milling Abutment + 1 Abutment Screw.
- > For Screw-Cement or Cement Retained Prosthesis.
- > Block abutment for customized contouring.
- > Gold color for more translucent restoration.
- > Connected with the Abutment Screw (2SSHR100).
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 30N.cm.
- > Fixture level impression.


Easy Temporary Abutment



Type	Hex		N-Hex	
Diameter	Ø4.5	Ø5.5	Ø4.5	Ø5.5
Length Cuff	10	10	10	10
2	2STHA45C	2STHA55C	2STNA45C	2STNA55C

- > Packing unit: 1 Easy Temporary Abutment + 1 Abutment Screw.
- > For Screw Retained Prosthesis.
- > For simpler and speedier chair-side process.
- > Venerable polymer material.
- > Temporary restoration for the anterior esthetic zone.
- > Titanium core for strength.
- > Connected with the Abutment Screw (2SSHR200).
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 20N.cm.
- > Fixture level impression.


Temporary Abutment



Type	Hex	N-Hex
Diameter	Ø4.5	Ø4.5
Length	10	10
Cuff		
1	2STHA45	2STNA45

- > Packing unit: 1 Temporary Abutment + 1 Abutment Screw.
- > For Screw-Cement Retained Prosthesis.
- > For provisional restoration.
- > Connected with the Abutment Screw (2SSHR100).
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 20N.cm.
- > Fixture level impression.


Abutment Screw



Diameter	Ø2.45	Ø2.15
Height	8.5	8.5
	2SSHR100	2SSHR200

- > Packing unit: 1 Abutment Screw.
- > 2SSHR100: Angulated, Milling, Temporary, Meta G UCLA, and Plastic UCLA Abutment.
- > 2SSHR200: Cemented and Easy Temporary Abutment.
- > Tightened with the 1.2 Hex Driver and Torque Wrench.


Meta G UCLA Abutment



Type	Hex	N-Hex
Diameter	Ø4.5	Ø4.5
Length	12	12
Cuff		
1	2SGH45N	2SGN45N
2	2SGH452N	2SGN452N
3	2SGH453N	2SGN453N

- > Packing unit: 1 Meta G UCLA Abutment + 1 Abutment Screw.
- > For Screw-Cement or Screw Retained Prosthesis.
- > Modification to the angulated abutment, customized abutment, and telescopic abutment.
- > CCM alloy core for precise connection.
- > Cast with non-precious metal or gold alloy.
- > Connected with the Abutment Screw (2SSHR100).
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 30N.cm.
- > Fixture level impression.


Replica



Diameter	Ø4
Height	12
	2SRHR001

- > Packing unit: 1 Replica.
- > Mimicking of the conical interface of the fixture.
- > Analog of fixture for the working cast.


Plastic UCLA Abutment



Type	Hex		N-Hex	
Diameter	Ø4.5	Ø5.5	Ø4.5	Ø5.5
Length	11	11	11	11
Cuff				
3	2SPHR001	2SPHW001	2SPNR001	2SPNW001

- > Packing unit: 1 Plastic UCLA Abutment + 1 Abutment Screw.
- > Same purpose of use as the Meta G UCLA Abutment but the low accuracy of connection during lab procedure.
- > PMMA material.
- > Connected with the Abutment Screw (2SSHR100).
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: Finger light force during wax pattern fabrication, 30N.cm after casting.
- > Fixture level impression.


Bite Impression Coping



Type	Hex(Short)	Hex(Long)	Hex(X-Long)	
Diameter	Ø4.5	Ø4.5	Ø4.5	
Cuff	2	4	6	
Length	4.0	2SBIC45S	2SBIC45L	2SBIC45X

- > Packing unit: 1 Bite Impression Coping (Inbuilt Guide Pin).
- > Designed to simultaneously take bite and impression.
- > For closed tray impression (Bite Impression).
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 12~15N.cm.


Pick-up Impression Coping



Type	Hex			N-Hex		
	Ø4.5	Ø5.5	Ø6.5	Ø4.5	Ø5.5	Ø6.5
12 (Short) / 4	2SIH454S	2SIH554S	2SIH654S	2SIN454S	2SIN554S	2SIN654S
14 (Short) / 2	2SIH45S	2SIH55S	2SIH65S	2SIN45S	2SIN55S	2SIN65S
16 (Long) / 4	2SIH45L	2SIH55L	2SIH65L	2SIN45L	2SIN55L	2SIN65L

- > Packing unit: 1 Pick-up Impression Coping + 1 Guide Pin.
- > For open tray impression.
- > Connected with the Guide Pin (2SISR001SS / 2SISR001SL).
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 12~15N.cm.

Transfer Post




Type	Hex			N-Hex		
	Ø4.5	Ø5.5	Ø6.5	Ø4.5	Ø5.5	Ø6.5
9 (Short) / 2	2STH45S	2STH55S	2STH65S	2STN45S	2STN55S	2STN65S
11 (Long) / 4	2STH45L	2STH55L	2STH65L	2STN45L	2STN55L	2STN65L


- > Packing unit: Hex - 1 Transfer Post + 1 Guide Pin / N-Hex - 1 Transfer Post (Solid Type).
- > For closed tray impression.
- > Connected with the Guide Pin (2STH001SS / 2STH001SL).
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 12~15N.cm.

Prosthetic Procedure II

Component Selection Guide for Multi S&A Abutment

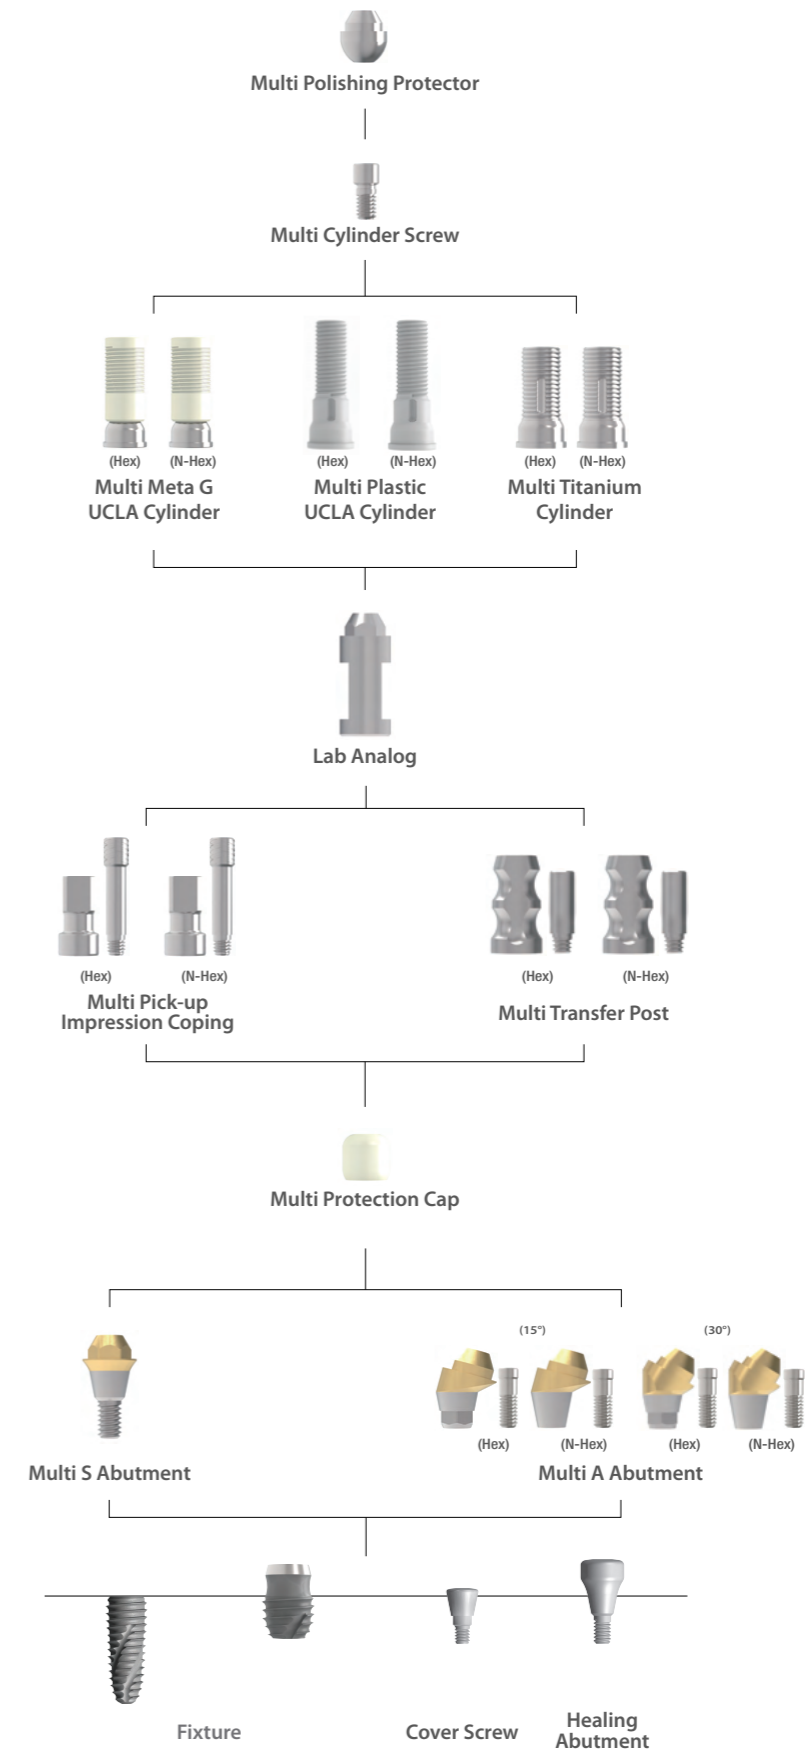


Multi S Abutment



Diameter	Ø4.5	Ø5.5
Cuff Length	2	2
1	2SMS451	2SMS551
2	2SMS452	2SMS552
3	2SMS453	2SMS553
4	2SMS454	2SMS554
5	2SMS455	2SMS555

- > Packing unit: 1 Multi S Abutment.
- > For Screw-Retained Prosthesis.
- > Titanium base for the cylinders.
- > Gold color for more translucent restoration.
- > Integrated with screw and abutment.
- > Library available for EXOCAD®, 3Shape® & Others.
- > Use the S Holder for a more stable position.
- > Tightened with the S Machine & S Ratchet Driver and Torque Wrench.
- > Tightening torque force: 30N.cm.
- > Abutment level impression.

Multi A Abutment




Type	Hex			
Diameter(Angle)	Ø4.5(15°)	Ø4.5(30°)	Ø5.5(15°)	Ø5.5(30°)
Cuff Length	2	2	2	2
2	● 2SMAH45152			
3	★ 2SMAH45153	● 2SMAH45303	★ 2SMAH55153	★ 2SMAH55303
4	★ 2SMAH45154	★ 2SMAH45304	★ 2SMAH55154	★ 2SMAH55304
5			★ 2SMAH55155	★ 2SMAH55305

Type	N-Hex			
Diameter(Angle)	Ø4.5(15°)	Ø4.5(30°)	Ø5.5(15°)	Ø5.5(30°)
Cuff Length	2	2	2	2
2	● 2SMAN45152			
3	★ 2SMAN45153	● 2SMAN45303	★ 2SMAN55153	★ 2SMAN55303
4	★ 2SMAN45154	★ 2SMAN45304	★ 2SMAN55154	★ 2SMAN55304
5			★ 2SMAN55155	★ 2SMAN55305

- > Packing unit: 1 Multi A Abutment + 1 Abutment Screw.
- > For Screw-Retained Prosthesis.
- > Titanium base for the cylinders.
- > Gold color for more translucent restoration.
- > Library available for EXOCAD®, 3Shape® & others.
- > Use the A Holder for a more stable position.
- > Connected with the Abutment Screw (2SSHR300: ★ / 2SSHR400: ●).
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 30N.cm.
- > Use the Multi Scanbody for digital flow.
- > Abutment level impression.


Abutment Screw



Height	7.5	6.5
Diameter	★ 2SSHR300	● 2SSHR400

- > Packing unit: 1 Abutment Screw.
- > To connect the Multi A Abutment.
- > Tightened with the 1.2 Hex Driver and Torque Wrench.


Multi Protection Cap



Multi S & A Abutment Diameter	Ø4.5	Ø5.5
Diameter	Ø5.2	Ø6.2
Height	5	5
	2SMPC45	2SMPC55

- > Packing unit: 1 Multi Protection Cap.
- > Protection from cheek and tongue for gingival healing period.
- > Gingival retraction for prosthodontic margin of the abutment.
- > Alternative usage for sub-structure of the temporary prosthesis.
- > Tightened with the 1.2 Hex Driver.
- > Tightening torque force: 5~10N.cm.


Multi Pick-up Impression Coping



Type	Hex		N-Hex	
Multi S & A Abutment Diameter	Ø4.5	Ø5.5	Ø4.5	Ø5.5
Diameter	Ø4.65	Ø5.65	Ø4.65	Ø5.65
Height	14.8	14.8	14.8	14.8
	2SMIH45	2SMIH55	2SMIN45	2SMIN55

- > Packing unit: 1 Multi Pick-up Impression Coping + 1 Guide Pin.
- > For open tray impression.
- > Connected with the Guide Pin (2SMGP012).
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 12~15N.cm.


Multi Transfer Post



Type	Hex		N-Hex	
Multi S & A Abutment Diameter	Ø4.5	Ø5.5	Ø4.5	Ø5.5
Diameter	Ø4.5	Ø5.5	Ø4.5	Ø5.5
Height	8.5	8.5	8.5	8.5
	2SMTH45	2SMTH55	2SMTN45	2SMTN55

- > Packing unit: 1 Multi Transfer Post + 1 Guide Pin.
- > For closed tray impression.
- > Connected with the Guide Pin (2SMTHS100).
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 12~15N.cm.


Multi Lab Analog



Type	Hex	N-Hex
Multi S & A Abutment Diameter	Ø4.5	Ø5.5
Diameter	Ø4.5	Ø5.5
Length	2	2
Cuff	2SMA45	2SMA55

- > Packing unit: 1 Multi Lab Analog.
- > Replacement of abutment shape in working cast.
- > Choose by abutment size.


Multi Titanium Cylinder



Type	Hex		N-Hex	
Multi S & A Abutment Diameter	Ø4.5	Ø5.5	Ø4.5	Ø5.5
Diameter	Ø4.5	Ø5.5	Ø4.5	Ø5.5
Length	8.5	8.5	8.5	8.5
Cuff	0.5	2STCH45	2STCH55	2STCN45
			2STCN45	2STCN55

- > Packing unit: 1 Multi Titanium Cylinder + 1 Multi Cylinder Screw.
- > For Screw, Cement or Screw-Cement Retained Prosthesis.
- > Connected with the Multi Cylinder Screw (2SMCS100).
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 20N.cm.


Multi Meta G UCLA Cylinder



Type	Hex		N-Hex	
Multi S & A Abutment Diameter	Ø4.5	Ø5.5	Ø4.5	Ø5.5
Diameter	Ø4.5	Ø5.5	Ø4.5	Ø5.5
Length	10.9	10.9	10.9	10.9
Cuff	0.5	2SCCH45	2SCCH55	2SCCN45
			2SCCN45	2SCCN55

- > Packing unit: 1 Multi Meta G UCLA Cylinder + 1 Multi Cylinder Screw.
- > For Screw, Cement, or Screw-Cement Retained Prosthesis.
- > Modification to various types of abutments.
- > CCM alloy core for precise connection.
- > Cast with non-precious metal or gold alloy.
- > Connected with the Multi Cylinder Screw (2SMCS100).
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 20N.cm.


Multi Cylinder Screw



Diameter	Ø2.25
Height	5
	2SMCS100

- > Packing unit: 1 Multi Cylinder Screw.
- > Connected with the Meta G UCLA, Plastic UCLA, and Titanium Cylinder.
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 20N.cm.


Multi Plastic UCLA Cylinder



Type	Hex		N-Hex	
Multi S & A Abutment Diameter	Ø4.5	Ø5.5	Ø4.5	Ø5.5
Diameter	Ø4.5	Ø5.5	Ø4.5	Ø5.5
Length	11.5	11.5	11.5	11.5
Cuff	0.5	2SMPH45	2SMPH55	2SMPN45
			2SMPN45	2SMPN55

- > Packing unit: 1 Multi Plastic UCLA Cylinder + 1 Multi Cylinder Screw.
- > For Screw, Cement or Screw-Cement Retained Prosthesis.
- > Same purpose of use as the Meta G UCLA Cylinder but the low accuracy of connection.
- > PMMA material.
- > Connected with the Multi Cylinder Screw (2SMCS100).
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 20N.cm.


Multi Polishing Protector




Type	Hex	
Multi S & A Abutment Diameter	Ø4.5	Ø5.5
Diameter	Ø4.5	Ø5.5
Length	2	2
	2SMPP45	2SMPP55

- > Packing unit: 1 Multi Polishing Protector.
- > To protect margin of the prosthesis while polishing procedure.

Multi Holder




S Holder



Type	Hand
Height 20	KMHS01

- > Packing unit: 1 Multi S Holder.
- > To position the Multi S Abutment more stably.



A Holder


Type	Hand
Height 32	KMHA01

- > Packing unit: 1 Multi A Holder.
- > To position the Multi A Abutment more stably.




- Connect the Multi A Holder with the Multi A Abutment with its Abutment Screw in it and match the direction of holes of the abutment and the holder.
- Hold the handle of the Multi A Holder and bend it according to the placement position in the oral cavity.
- Connect the assembled body with the fixture.
- Tighten the Multi Abutment with the 1.2 Hex Driver and Torque Wrench.

Multi S Machine Driver




Type	Machine
Height 27.5	KMMSD21L

- > Packing unit: 1 Multi S Machine Driver.
- > To install and remove the Multi S Abutment by machine.




Multi S Ratchet Driver




Type	Ratchet
Height 22	KRMSD15L

- > Packing unit: 1 Multi S Ratchet Driver.
- > To install and remove the Multi S Abutment with the Torque Wrench.




Prosthetic Procedure III

Component Selection Guide for Lock Abutment




Lock Abutment



Diameter	Ø3.5
Cuff Length	2.15
0.5	2SLA400
1	2SLA410
2	2SLA420
3	2SLA430
4	2SLA440

- > Packing unit: 1 Lock Abutment.
- > For Screw-Retained Prosthesis.
- > Titanium base for the cylinders.
- > Gold color for more translucent restoration.
- > Integrated with screw and abutment.
- > Tightened with the Lock Ratchet Driver and Torque Wrench.
- > Tightening torque force: 30N.cm.
- > Abutment level impression.


Lock Protection Cap



Lock Abutment Diameter	Ø3.5
Diameter	Ø4.3
Height	4
4	2SLP45

- > Packing unit: 1 Lock Protection Cap.
- > Protection from cheek and tongue for gingival healing period.
- > Gingival retraction for prosthodontic margin of the abutment.
- > Tightened with the 1.2 Hex Driver.
- > Tightening torque force: 5~10N.cm.

Lock Pick-up Impression Coping



Lock Abutment Diameter	Ø3.5
Diameter	Ø4.3
Height	16
16	2SLIH45

- > Packing unit: 1 Lock Pick-up Impression Coping + 1 Guide Pin.
- > Connected with the Guide Pin (2SLIH45S).
- > For open tray impression.


Lock Lab Analog



Lock Abutment Diameter	Ø3.5
Diameter	Ø3.5
Length	2.15
2.15	2SLA45

- > Packing unit: 1 Lock Lab Analog.
- > Replacement of abutment shape in working cast.
- > Tightened with the 1.2 Hex Driver and Torque Wrench.


Lock Meta G UCLA Cylinder



Lock Abutment Diameter	Ø3.5
Diameter	Ø4.3
Height	11.2
11.2	2SLCH45

- > Packing unit : 1 Lock Meta G UCLA Cylinder + 1 Lock Cylinder Screw.
- > For Screw, Cement, or Screw-Cement Retained Prosthesis.
- > Modification to various types of abutments.
- > CCM alloy core for precise connection.
- > Cast with non-precious metal or gold alloy.
- > Connected with the Lock Cylinder Screw (2SLCS200).
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 30N.cm.


Lock Titanium Cylinder



Lock Abutment Diameter	Ø3.5
Diameter	Ø4.3
Height	10
10	2SLTH45

- > Packing unit: 1 Lock Titanium Cylinder + 1 Lock Cylinder Screw.
- > For Screw, Cement, or Screw-Cement Retained Prosthesis.
- > Connected with the Lock Cylinder Screw (2SLCS200).
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force : 30N.cm.



Lock Cylinder Screw



Diameter	Ø2.3
Height	2SLCS200

- > Packing unit: 1 Lock Cylinder Screw.
- > Connected with the CCM Cylinder and Titanium Cylinder.
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 30N.cm.

Lock Ratchet Driver




Type	Ratchet
Height 14.2	KRLRD18
Height 28.5	KRLRD28

- > Packing unit: 1 Lock Ratchet Driver.
- > To install and remove the Lock Abutment with the Torque Wrench.




Prosthetic Procedure IV

Component Selection Guide for Absolute Abutment

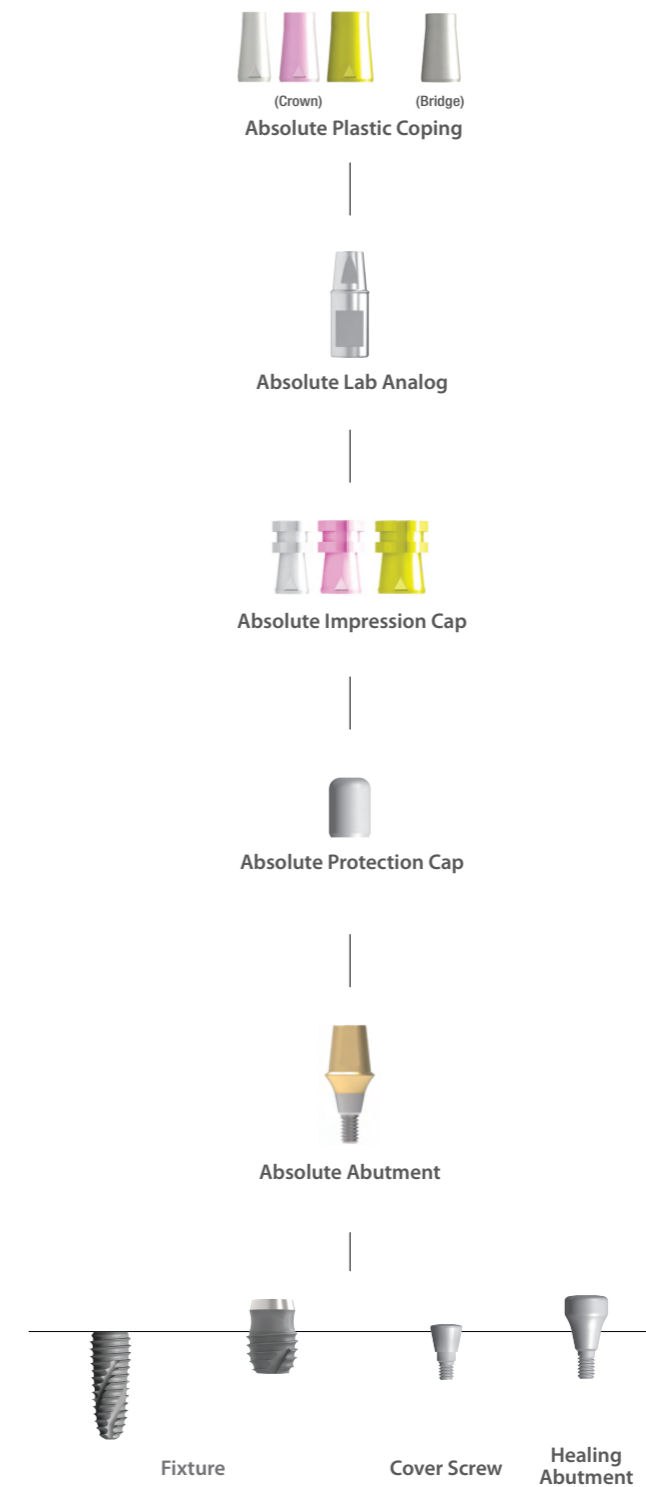


Absolute Abutment



Diameter Length Cuff	Ø4.5			Ø5.5			Ø6.5		
	4	5.5	7	4	5.5	7	4	5.5	7
1	2SAC4514	2SAC4515	2SAC4517	2SAC5514	2SAC5515	2SAC5517	2SAC6514	2SAC6515	2SAC6517
2	2SAC4524	2SAC4525	2SAC4527	2SAC5524	2SAC5525	2SAC5527	2SAC6524	2SAC6525	2SAC6527
3	2SAC4534	2SAC4535	2SAC4537	2SAC5534	2SAC5535	2SAC5537	2SAC6534	2SAC6535	2SAC6537
4	2SAC4544	2SAC4545	2SAC4547	2SAC5544	2SAC5545	2SAC5547	2SAC6544	2SAC6545	2SAC6547
5	2SAC4554	2SAC4555	2SAC4557	2SAC5554	2SAC5555	2SAC5557	2SAC6554	2SAC6555	2SAC6557

- > Packing unit: 1 Absolute Abutment + 1 Protection Cap.
- > For Cement Retained Prosthesis.
- > Cutting surface for anti-rotation of the prosthesis.
- > Integrated with the Screw and Abutment.
- > Tightened with the 1.2 Hex Driver or the Absolute Ratchet Driver and Torque Wrench.
- > Tightening torque force: 30N.cm.
- > Abutment level impression.


Absolute Ratchet Driver



Diameter Length Height	Ø4.6		Ø5.6		Ø6.6	
	12	19	12	19	12	19
19	KRAD4512S		KRAD5512S		KRAD6512S	
26	KRAD4519L		KRAD5519L		KRAD6519L	

- > Packing unit: 1 Absolute Ratchet Driver.
- > To install and remove the Absolute with the Torque Wrench.


Absolute Protection Cap



Absolute Abutment Diameter Height	Ø4.5		Ø5.5		Ø6.5	
	Diameter	Height	Diameter	Height	Diameter	Height
6	2SHPC454		2SHPC554		2SHPC654	
7.5	2SHPC455		2SHPC555		2SHPC655	
9	2SHPC457		2SHPC557		2SHPC657	

- > Packing unit: 1 Absolute Protection Cap.
- > Protection from cheek and tongue for gingival healing period.
- > Gingival retraction for prosthodontic margin of the abutment.
- > Alternative usage for sub-structure of the temporary prosthesis.


Absolute Impression Cap



Absolute Abutment Diameter Height	Ø4.5		Ø5.5		Ø6.5	
	Diameter	Height	Diameter	Height	Diameter	Height
10.3	2SIC45		2SIC55		2SIC65	

- > Packing unit: 1 Absolute Impression Cap.
- > Confirm locking with abutment by rotation of clockwise and anti-clockwise direction.


Absolute Lab Analog



Absolute Abutment Diameter Length	Ø4.5		Ø5.5		Ø6.5	
	Diameter	Length	Diameter	Length	Diameter	Length
4.1	2SHLA454		2SHLA554		2SHLA654	
5.6	2SHLA455		2SHLA555		2SHLA655	
7.1	2SHLA457		2SHLA557		2SHLA657	

- > Packing unit: 1 Absolute Lab Analog.
- > Replacement of abutment shape in working cast.
- > Choose according to width and length of the abutment.

Absolute Plastic Coping (Burn Out Cylinder)



Type	Crown			Bridge		
	Absolute Abutment Diameter	Diameter	Height	Absolute Abutment Diameter	Diameter	Height
10	Ø4.5	Ø5.1	10	Ø4.5	Ø5.1	10
	Ø5.5	Ø6.1	10	Ø5.5	Ø6.1	10
	Ø6.5	Ø7.1	10	Ø6.5	Ø7.1	10


- > Packing unit: 1 Absolute Plastic Coping.
- > Connected with the Lab Analog.
- > Burn out and casting for the metal framework.

Prosthetic Procedure V


Component Selection Guide for Straight Abutment



Straight Abutment




Straight Abutment



Diameter Length Cuff	Ø3.5		Ø4.5	
	Diameter	Length	Diameter	Length
0.5	2SSCM308		2SSCR408	
1	2SSCM318		2SSCR418	
2	2SSCM328		2SSCR428	
3	2SSCM338		2SSCR438	
4	2SSCM348		2SSCR448	

- > Packing unit: 1 Straight Abutment.
- > For Cement Retained Prosthesis.
- > Integrated with screw and abutment.
- > Tightened with the Shoulder Driver.
- > Tightening torque force: 30N.cm.
- > Direct impression.

Shoulder Driver




Diameter Height	Ø4.5	
	Diameter	Height
19	KRR19L	


- > Packing unit: 1 Driver.
- > To install and remove the Straight Abutment with the Torque Wrench.

Prosthetic Procedure VI



Component Selection Guide for Sonator S&A Abutment



Sonator S Abutment




Carrier





Diameter	Ø4.0					
Length	1	2	3	4	5	6
Cuff	SONS401	SONS402	SONS403	SONS404	SONS405	SONS406

- > Packing unit: 1 Sonator S Abutment + 1 Carrier + 3 H-Type Inner Caps + 1 Outer Cap + 1 Block-out Spacer + 1 Black Processing Male.
- > For Implant-Supported Overdenture Prosthesis.
- > Stable with low vertical height.
- > 6 kinds of Inner Caps give various holding force (Both, H and NH-Type Inner Caps are used for the Sonator S Abutment).
- > Path compensation up to 20° based on 2 implants.
- > Carrier: Used for delivery of the abutment.
- > Tightened with the Sonator S Ratchet Driver and Torque Wrench.
- > Tightening torque force: 30N.cm.
- > Abutment level impression.

Sonator A Abutment



Carrier



Diameter	Ø4.0	
Length	1.5	3.0
Angle	3	
Cuff	SONA415	SONA430

- > Packing unit: 1 Sonator A Abutment + 1 Abutment Screw + 1 Carrier + 3 NH-Type Inner Caps + 1 Outer Cap + 1 Block-out Spacer + 1 Black Processing Male.
- > For Implant-Supported Overdenture Prosthesis.
- > Stable with low vertical height.
- > 6 kinds of Inner Caps give various holding force (Both, H and NH-Type Inner Caps are used for the Sonator A Abutment).
- > Path compensation up to 40° based on 2 Implants.
- > Connected with the Abutment Screw (2SSHR300).
- > Carrier: Used for delivery of the abutment.
- > Tightened with the 1.2 Hex Driver and Torque wrench.
- > Tightening torque force: 30N.cm.
- > Abutment level impression.


Abutment Screw



Diameter	Ø2.15
Height	7.5
	2SSHR300

- > Packing unit: 1 Abutment Screw.
- > To connect the Sonator A Abutment.
- > Tighten with the 1.2 Hex Driver and Torque Wrench.

Outer Cap



Diameter	Ø5.4
Height	2.25
SONOC01	

- > Packing unit: 2 Outer Caps and 2 Black Processing Males.
- > Black Processing Male: Inserted and removed with the I&R Driver.


Sonator Lab Analog



Diameter	Ø4
Length	1.4
SONLA04	

- > Packing unit: 4 Sonator Lab Analogs.
- > Replacement of abutment shape in working cast.


H-Type Inner Cap

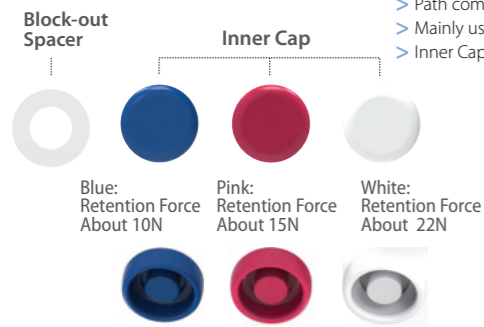

Code	SONIC01
-------------	---------

- > Packing unit: 3 Block-out Spacers + 3 Inner Caps (1 Blue, 1 Pink, and 1 White).
- > Path compensation up to 20° based on 2 implants.
- > Mainly used for the Sonator S Abutment.
- > Inner Caps: Inserted and removed with the I&R Driver.


NH-Type Inner Cap



Code	SONIC02
-------------	---------

- > Packing unit: 3 Block-out Spacers + 3 Inner Caps (1 Red, 1 Orange, and 1 Green).
- > Non-humped design.
- > Path compensation up to 40° based on 2 implants.
- > Mainly used for the Sonator A Abutment.
- > Inner Caps: Inserted and removed with the I&R Driver.


Sonator Impression Coping



Diameter	Ø4.8
Length	3
SONIP04	

- > Packing unit: 4 Sonator Impression Copings and 4 Black Processing Males.
- > Connected over the Sonator S&A Abutment after placing the Block-out Spacer.
- > For close tray impression.


Sonator S Ratchet Driver



Type	Ratchet
Height	18
SONRD19L	

- > Packing unit : 1 Sonator S Ratchet Driver.
- > To install and remove the Sonator S Abutment with the Torque Wrench.

Sonator I&R Driver




Height	95.4
SONIR002	


- > Packing unit: 1 Sonator I&R Driver.
- > Used to insert and remove the Inner Caps and Block Processing Male.

Prosthetic Procedure VII


Component Selection Guide for Ball Abutment

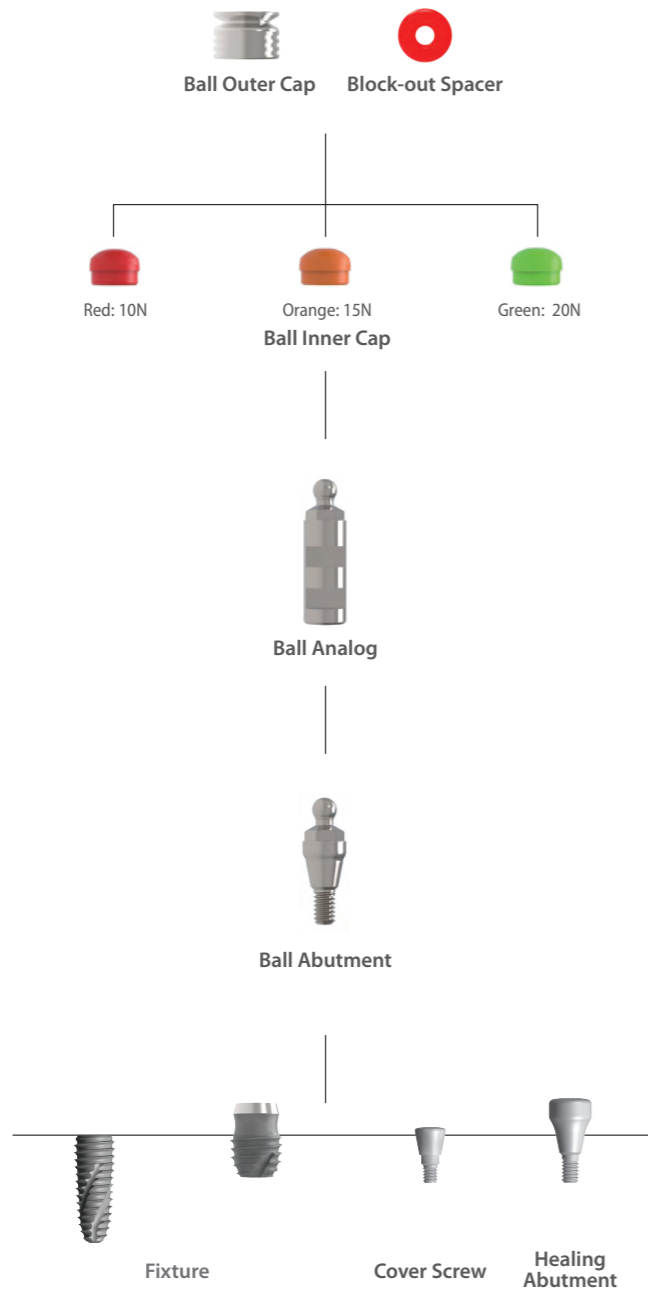

Ball Abutment



Ball Inner Cap




Ball Abutment

Diameter	Ø4.0
Length	4
Cuff	
1	2SBAT414R
2	2SBAT424R
3	2SBAT434R
4	2SBAT444R
5	2SBAT454R

- > Packing unit: 1 Ball Abutment + 3 Inner Caps (1 per each colour) + 1 Block-out Spacer + 1 Outer Cap.
- > For Implant-Supported Overdenture Prosthesis.
- > Tightened with the Ball Driver and Torque Wrench.
- > Tightening torque force: 30N.cm.
- > Direct impression.


Ball Outer Cap



Diameter	Ø3.4
Height	2.4
	BATC003C

- > Packing unit: 2 Outer Caps.

Ball Inner Cap



	BATC003I
--	----------

- > Packing unit: 2 Block-out Spacers + 6 Inner Caps (2 per each color).
- > Retention force: Red 10N, Orange 15N & Green 20N.


Ball Analog



Diameter	Ø4.0
Length	4
	SBAL400

- > Packing unit: 4 Lab Analogs.
- > Replacement of abutment shape in working cast.

Ball Driver




Height	Type	Ratchet
19		KRB19L

- > Packing unit: 1 Ball Driver.
- > To install and remove the Ball Abutment with the Torque Wrench.

*Extra Product

Ball I&R Driver












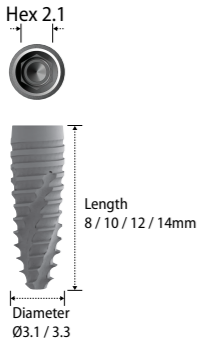






Height	100
	KBIR01




- > Packing unit: 1 Ball I&R Driver.
- > Used to insert and remove the Inner Caps into and out of the Outer Cap.

INNO SUBMERGED NARROW IMPLANT (Sub-N.)

System Flow

Fixture	Abutment	Impression
	<p>Prosthetic Procedure I</p> <div style="display: flex; justify-content: space-around; align-items: flex-start;"> <div style="text-align: center;"> <p>065p</p>  <p>Cemented Abutment</p> </div> <div style="text-align: center;"> <p>065p</p>  <p>Angulated Abutment</p> </div> <div style="text-align: center;"> <p>065p</p>  <p>Temporary Abutment</p> </div> <div style="text-align: center;"> <p>066p</p>  <p>Meta G UCLA Abutment</p> </div> </div>	<p>Fixture Level Impression</p> <div style="display: flex; justify-content: space-around; align-items: flex-start;"> <div style="text-align: center;"> <p>066p</p>  <p>Replica</p> </div> <div style="text-align: center;"> <p>067p</p>  <p>Pick-up Impression Coping</p> </div> <div style="text-align: center;"> <p>067p</p>  <p>Transfer Post</p> </div> </div>
	<p>Prosthetic Procedure II</p> <div style="display: flex; justify-content: space-around; align-items: flex-start;"> <div style="text-align: center;"> <p>063p</p>  <p>Multi S Abutment</p> </div> <div style="text-align: center;"> <p>063p</p>  <p>Multi A Abutment</p> </div> <div style="text-align: center;"> <p>071p</p>  <p>Multi Meta G ULCA Cylinder</p> </div> <div style="text-align: center;"> <p>071p</p>  <p>Multi Plastic UCLA Cylinder</p> </div> <div style="text-align: center;"> <p>072p</p>  <p>Multi Titanium Cylinder</p> </div> </div>	<p>Abutment Level Impression</p> <div style="display: flex; justify-content: space-around; align-items: flex-start;"> <div style="text-align: center;"> <p>070p</p>  <p>Multi Protection Cap</p> </div> <div style="text-align: center;"> <p>070p</p>  <p>Multi Pick-up Impression Coping</p> </div> <div style="text-align: center;"> <p>070p</p>  <p>Multi Transfer Post</p> </div> <div style="text-align: center;"> <p>071p</p>  <p>Multi Lab Analog</p> </div> </div>
	<p>Prosthetic Procedure III</p> <div style="text-align: center;"> <p>074p</p>  <p>Straight Abutment</p> </div>	<p>Direct Impression</p>

INNO Submerged Narrow Implant (Sub-N.)




Submerged Fixture
Surface Treatment: **SLA-SH™**

- > Interchangeable with hexagonal Morse tapered fixture.
- > Internal hex connection (Taper 11°/ Hex 2.1).

※ Note


> The INNO Sub. Narrow System is not compatible with the INNO Submerged System as hexagon size is different.



No-Mount > Packing unit: 1 Fixture + 1 Cover Screw.


Diameter **Ø3.1**
Length

8	SR3108NSM
10	SR3110NSM
12	SR3112NSM
14	SR3114NSM



Diameter **Ø3.3**
Length


8	SR3308NSM
10	SR3310NSM
12	SR3312NSM
14	SR3314NSM



Pre-Mount > Packing unit: 1 Fixture + 1 Cover Screw + 1 Mount.


Diameter **Ø3.1**
Length

8	SR3108NS
10	SR3110NS
12	SR3112NS
14	SR3114NS



Diameter **Ø3.3**
Length

8	SR3308NS
10	SR3310NS
12	SR3312NS
14	SR3314NS



Fixture Mount



Length	5.4
	RSM001

- > Packing unit: 1 Mount + 1 Mount Screw.
- > Tightened with the 1.2 Hex Driver.
- > Tightening torque force: 5~10N.cm.


Cover Screw



Diameter / Length	Ø2.85	Ø3.25	Ø3.6
1.7	RCS000		
2.7		RCS001	
3.7			RCS002

- > Packing unit: 1 Cover Screw.
- > To seal the conical interface of the fixture.
- > The longer the Cover Screw for the deeply inserted fixture.
- > Tightened with the 1.2 Hex Driver.
- > Tightening torque force: 5~10N.cm.

Healing Abutment




Diameter	Ø3.5		Ø4.5	
Cuff / Length	1	2	1	2
0.5	HR3501			
1	HR3511		HS4511N	
2		HR3522		HS4522N
3		HR3532		HS4532N
4		HR3542		HS4542N
5				HS4552N
7				HS4572N


- > Packing unit: 1 Healing Abutment.
- > For remodeling gingival contour during soft tissue healing.
- > Select the abutment according to gingival height and abutment type.
- > Tightened with the 1.2 Hex Driver.
- > Tightening torque force: 5~10N.cm.

Prosthesis Procedure I

Components Selection Guide for Cemented and UCLA Abutment

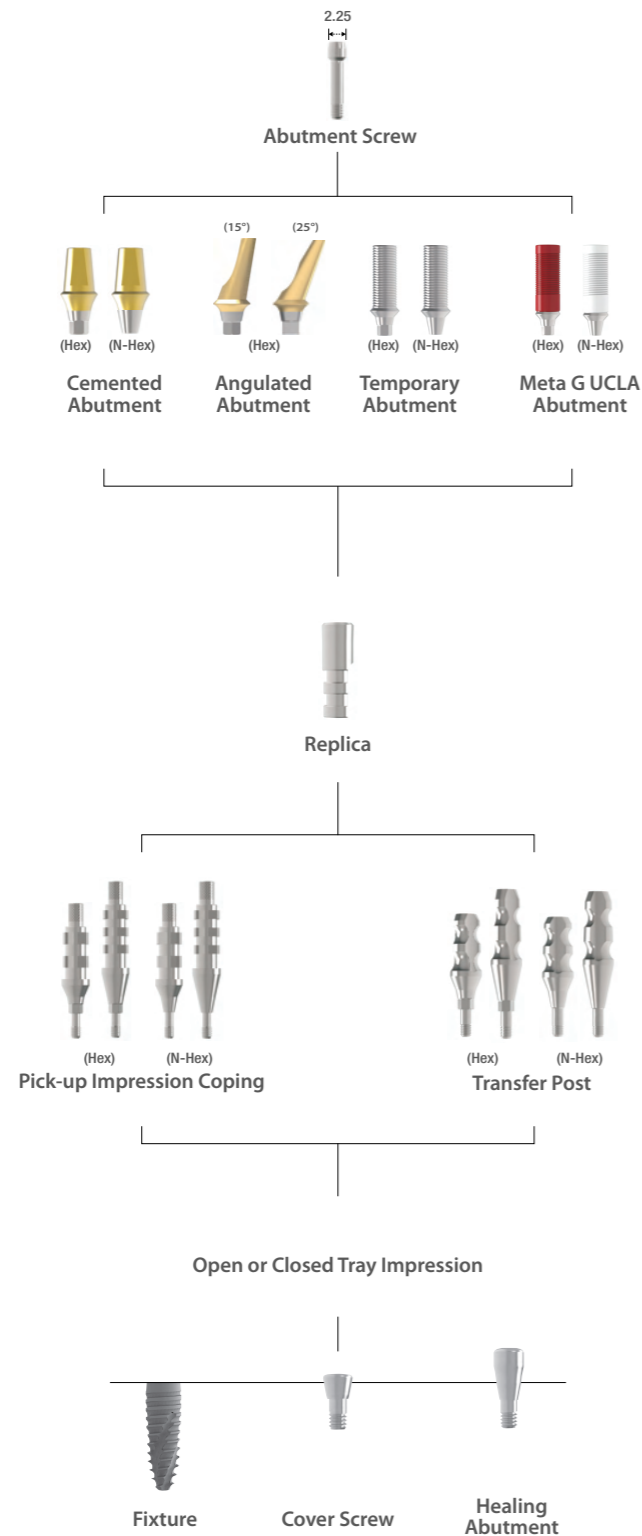


Cemented Abutment



Type	Hex			N-Hex		
Diameter	Ø4.5					
Length	4	5.5	7	4	5.5	7
1	SCH4514N	SCH4515N	SCH4517N	SCN4514N	SCN4515N	SCN4517N
2	SCH4524N	SCH4525N	SCH4527N	SCN4524N	SCN4525N	SCN4527N
3	SCH4534N	SCH4535N	SCH4537N	SCN4534N	SCN4535N	SCN4537N
4	SCH4544N	SCH4545N	SCH4547N	SCN4544N	SCN4545N	SCN4547N
5	SCH4554N	SCH4555N	SCH4557N	SCN4554N	SCN4555N	SCN4557N

- > Packing unit: 1 Cemented Abutment + 1 Abutment Screw.
- > For Screw-Cement or Cement Retained Prosthesis.
- > Cutting surface for anti-rotation of the prosthesis.
- > Gold color for more translucent restoration.
- > Library available for EXOCAD®, 3Shape® & Others.
- > Connected with the Abutment Screw (SSHR100N).
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 20~25N.cm.
- > Use the Scanbody for 3D Work.
- > Fixture level impression.


Angulated Abutment



Type	Hex	
Diameter(Angle)	Ø4.5(15°)	Ø4.5(25°)
Length	8	
1	SAH45151NA	SAH45251NA
2	SAH45152NA	SAH45252NA
3	SAH45153NA	SAH45253NA
4	SAH45154NA	SAH45254NA

- > Packing unit: 1 Angulated Abutment + 1 Abutment Screw.
- > For Screw-Cement or Cement Retained Prosthesis.
- > Solution for the anterior esthetic zone.
- > Gold color for esthetics.
- > Connected with the Abutment Screw (SSHR100N).
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 20~25N.cm.
- > Fixture level impression.


Temporary Abutment



Type	Hex	N-Hex
Diameter	Ø4.5	
Length	10	
1	STHA45N	STNA45N

- > Packing unit: 1 Temporary Abutment + 1 Abutment Screw.
- > For Screw-Cement Retained Prosthesis.
- > For provisional restoration.
- > Connected with the Abutment Screw (SSHR100N).
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 20~25N.cm.


Meta G UCLA Abutment



Type	Hex	N-Hex
Diameter	Ø4.5	Ø4.5
Length / Cuff	12	12
1	SGH45N	SGN45N
2	SGH452N	SGN452N
3	SGH453N	SGN453N

- > Packing unit: 1 Meta G UCLA Abutment + 1 Abutment Screw.
- > For Screw Retained Prosthesis.
- > Modification to the angulated abutment, customized abutment and telescopic abutment.
- > CCM alloy core for precise connection.
- > Cast with non-precious metal or gold alloy.
- > Connected with the Abutment Screw (SSHR100N).
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 20~25N.cm.
- > Fixture level impression.

Abutment Screw



Diameter	2.25
Height	10.2
	SSHR100N

- > Packing unit: 1 Abutment Screw.
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 20~25N.cm.


Replica



Diameter	Ø4
Height	12.1
	SRHR001N

- > Packing unit: 1 Replica.
- > Mimicking of the conical interface of the fixture.
- > Analog of fixture for the working cast.


Pick-up Impression Coping



Type	Hex	N-Hex
Diameter	Ø4.5	Ø4.5
Length / Cuff	14 (Short) / 2	14 (Short) / 2
	SIH45SN	SIN45SN
	16 (Long) / 4	16 (Long) / 4
	SIH45LN	SIN45LN

- > Packing unit: 1 Pick-up Impression Coping + 1 Guide Pin.
- > For open tray impression.
- > Connected with the Guide Pin (SIS001SN / SIS001LN).
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 12~15Ncm.

Transfer Post




Type	Hex	N-Hex
Diameter	Ø4.5	Ø4.5
Length / Cuff	9 (Short) / 2	9 (Short) / 2
	STH45SN	STN45SN
	11 (Long) / 4	11 (Long) / 4
	STH45LN	STN45LN


- > Packing unit: Hex - 1 Transfer Post + 1 Guide Pin / N-Hex - 1 Transfer Post (Solid Type).
- > For closed tray impression.
- > Connected with the Guide Pin (STS001SN / STS001LN).
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 12~15Ncm.

Prosthesis Procedure II

Component Selection Guide for Multi S&A Abutment

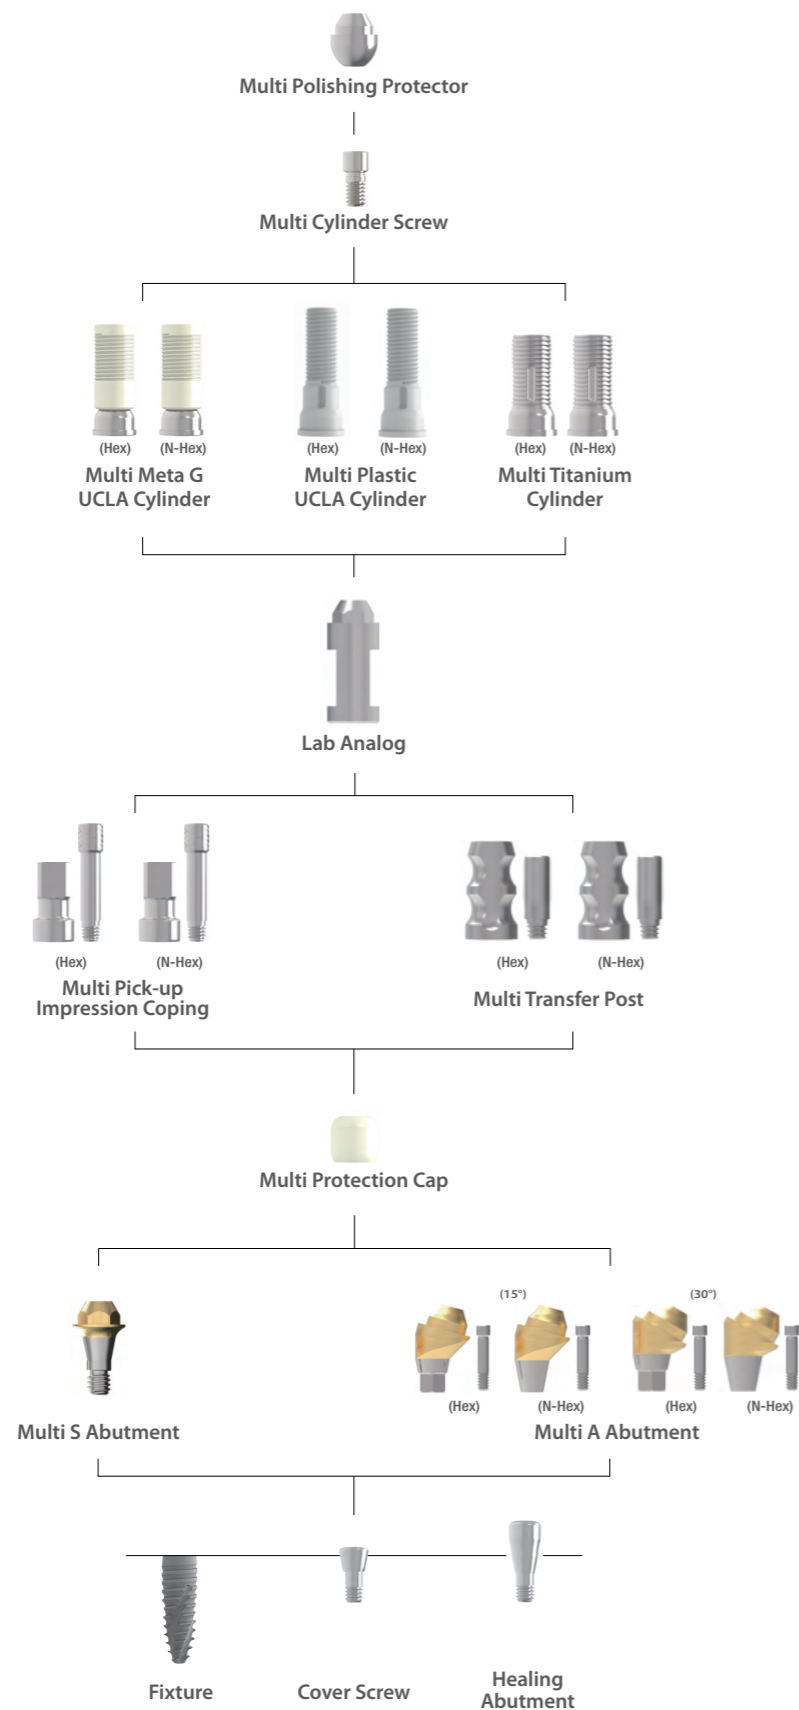


Multi S Abutment



Diameter	Ø4.5
Cuff Length	2
1	SMS451N
2	SMS452N
3	SMS453N
4	SMS454N

- > Packing unit: 1 Multi S Abutment.
- > For Screw-Retained Prosthesis.
- > Titanium base for the cylinders.
- > Gold color for more translucent restoration.
- > Integrated with screw and abutment.
- > Library available for EXOCAD®, 3Shape® & Others.
- > Use the S Holder for a more stable position.
- > Tightened with the S Machine & S Ratchet Driver and Torque Wrench.
- > Tightening torque force: 20~25N.cm.
- > Abutment level impression.

Multi A Abutment




Type	Hex	
Diameter(Angle)	Ø4.5(15°)	Ø4.5(30°)
Cuff Length	2	2
2	★ SMAH45152N	
3	● SMAH45153N	★ SMAH45303N
4	● SMAH45154N	● SMAH45304N

Type	N-Hex	
Diameter(Angle)	Ø4.5(15°)	Ø4.5(30°)
Cuff Length	2	2
2	★ SMAN45152N	
3	● SMAN45153N	★ SMAN45303N
4	● SMAN45154N	● SMAN45304N

- > Packing unit: 1 Multi A Abutment + 1 Abutment Screw.
- > For Screw-Retained Prosthesis.
- > Titanium base for the cylinders.
- > Gold color for more translucent restoration.
- > Library available for EXOCAD®, 3Shape® & Others.
- > Use the A Holder for a more stable position.
- > Connected with the Abutment Screw (SSHR200N: ★ / SSHR300N: ●).
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 20~25N.cm.
- > Abutment level impression.


Abutment Screw



Height	8.7	9.3
Diameter	Ø1.95	● SSHR300N
	★ SSHR200N	

- > Packing unit: 1 Abutment Screw.
- > To connect the Multi A Abutment.
- > Tightened with the 1.2 Hex Driver and Torque Wrench.


Multi Protection Cap



Multi S & A Abutment Diameter	Ø4.5
Diameter	Ø5.2
Height	5
2SMPC45	

- > Packing unit: 1 Multi Protection Cap.
- > Protection from cheek and tongue for gingival healing period.
- > Gingival retraction for prosthodontic margin of the abutment.
- > Alternative usage for sub-structure of the temporary prosthesis.
- > Tightened with the 1.2 Hex Driver.
- > Tightening torque force: 5~10N.cm.


Multi Lab Analog



Multi S & A Abutment Diameter	Ø4.5
Diameter	Ø4.5
Length	2
2SMA45	

- > Packing unit: 1 Multi Lab Analog.
- > Replacement of abutment shape in working cast.


Multi Pick-up Impression Coping



Type	Hex	N-Hex
Multi S & A Abutment Diameter	Ø4.5	Ø4.5
Diameter	Ø4.65	Ø4.65
Height	14.8	14.8
2SMIH45		2SMIN45

- > Packing unit: 1 Multi Pick-up Impression Coping + 1 Guide Pin.
- > For open tray impression.
- > Connected with the Guide Pin (2SMGP012).
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 12~15N.cm.


Multi Meta G UCLA Cylinder



Type	Hex	N-Hex
Multi S & A Abutment Diameter	Ø4.5	Ø4.5
Diameter	Ø4.5	Ø4.5
Length	10.9	10.9
Cuff	0.5	0.5
2SCCH45		2SCCN45

- > Packing unit: 1 Multi Meta G UCLA Cylinder + 1 Multi Cylinder Screw.
- > For Screw, Cement, or Screw-Cement Retained Prosthesis.
- > Modification to various types of abutments.
- > CCM alloy core for precise connection.
- > Cast with non-precious metal or gold alloy.
- > Connected with the Multi Cylinder Screw (2SMCS100).
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 20N.cm.


Multi Transfer Post



Type	Hex	N-Hex
Multi S & A Abutment Diameter	Ø4.5	Ø4.5
Diameter	Ø4.5	Ø4.5
Height	8.5	8.5
2SMTH45		2SMTN45

- > Packing unit: 1 Multi Transfer Post + 1 Guide Pin.
- > For closed tray impression.
- > Connected with the Guide Pin (2SMTHS100).
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 12~15N.cm.


Multi Plastic UCLA Cylinder



Type	Hex	N-Hex
Multi S & A Abutment Diameter	Ø4.5	Ø4.5
Diameter	Ø4.5	Ø4.5
Length	11.5	11.5
Cuff	0.5	0.5
2SMPH45		2SMPN45

- > Packing unit: 1 Multi Plastic UCLA Cylinder + 1 Multi Cylinder Screw.
- > For Screw, Cement or Screw-Cement Retained Prosthesis.
- > Same purpose of use as the Meta G UCLA Cylinder but the low accuracy of connection.
- > PMMA material.
- > Connected with the Multi Cylinder Screw (2SMCS100).
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 20N.cm.


Multi Titanium Cylinder



Type	Hex	N-Hex
Multi S & A Abutment Diameter	Ø4.5	Ø4.5
Diameter	Ø4.5	Ø4.5
Length	8.5	8.5
Cuff	0.5	2STCH45
		2STCN45

- > Packing unit: 1 Multi Titanium Cylinder + 1 Multi Cylinder Screw.
- > For Screw, Cement or Screw-Cement Retained Prosthesis.
- > Connected with the Multi Cylinder Screw (2SMCS100).
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 20N.cm.


Multi Cylinder Screw



Diameter	Ø2.25
Height	5
	2SMCS100

- > Packing unit: 1 Multi Cylinder Screw.
- > Connected with the Meta G UCLA, Plastic UCLA, and Titanium Cylinder.
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 20N.cm.



Multi Polishing Protector



Type	Hex
Multi S & A Abutment Diameter	Ø4.5
Diameter	Ø4.5
Length	2
	2SMPP45

- > Packing unit: 1 Multi Polishing Protector.
- > To protect margin of the prosthesis while polishing procedure.

Multi Holder



Height	Type	Hand
20		KMHS01

- > Packing unit: 1 Multi S Holder.
- > To position the Multi S Abutment more stably.



A Holder


Height	Type	Hand
32		KMHA01

- > Packing unit: 1 Multi A Holder.
- > To position the Multi A Abutment more stably.




- Connect the Multi A Holder with the Multi A Abutment with its Abutment Screw in it and match the direction of holes of the abutment and the holder.
- Hold the handle of the Multi A Holder and bend it according to the placement position in the oral cavity.
- Connect the assembled body with the fixture.
- Tighten the Multi Abutment with the 1.2 Hex Driver and Torque Wrench.

Multi S Machine Driver




Height	Type	Machine
27.5		KMMSD21L

- > Packing unit: 1 Multi S Machine Driver.
- > To install and remove the Multi S Abutment by machine.




Multi S Ratchet Driver




Height	Type	Ratchet
22		KRMSD15L

- > Packing unit: 1 Multi S Ratchet Driver.
- > To install and remove the Multi S Abutment with the Torque Wrench.




Prosthesis Procedure III

Component Selection Guide for Straight Abutment




Straight Abutment



Diameter	Ø3.5				
Length [Cuff]	8 [0.5]	8 [1]	8 [2]	8 [3]	8 [4]
	SR308	SR318	SR328	SR338	SR348


- > Packing unit: 1 Straight Abutment.
- > For Cement Retained Prosthesis.
- > Integrated with screw and abutment.
- > Tightened with the Shoulder Driver.
- > Tightening torque force: 20~25N.cm.
- > Direct impression.

Shoulder Driver














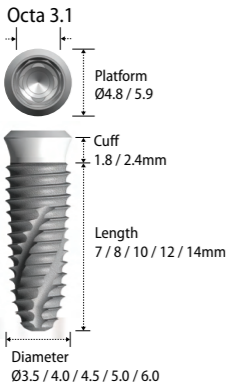











Diameter	Ø4.5
Height	19
	KRR19L

- > Packing unit: 1 Shoulder Driver.
- > To install and remove the Straight Abutment with the Torque Wrench.



INNO INTERNAL IMPLANT (Int.)

System Flow


Fixture	Abutment		Impression	
	Prosthetic Procedure I	  	Fixture Level Impression	  
	Prosthetic Procedure II		Abutment Level Impression	    
	Prosthetic Procedure III			   
	Prosthetic Procedure IV			 
	Prosthetic Procedure V			

INNO Internal Implant (Int.)



Internal Fixture
Surface Treatment: **SLA-SH™**

- > Interchangeable with 1 staged internal fixture.
- > Internal Octa Connection (Taper 8°/ Octa 3.1).
- > No-Mount type.



INNO Fixture Code

I	P	T	40	10	S	M	<i>*Ex.)</i>	
Type Internal	P=Cuff 1.8	body Taper	Diameter Ø4.0	Length 10mm	Surface Treatment SLA	Mount No-Mount	SLA Cuff 1.8 No-Mount	IP4010SM



I		T	40	10	S	M	<i>*Ex.)</i>	
Type Internal	Cuff 2.4	body Taper	Diameter Ø4.0	Length 10mm	Surface Treatment SLA	Mount No-Mount	SLA Cuff 2.4 No-Mount	IT4010SM

No-Mount Cuff 1.8mm fixture > Packing unit: 1 Fixture + 1 Cover Screw.

* Diameter **Ø3.5**

Length



7	-
8	IP3508SM
10	IP3510SM
12	IP3512SM
14	IP3514SM



* Diameter **Ø4.0**

Length



7	IP4007SM
8	IP4008SM
10	IP4010SM
12	IP4012SM
14	IP4014SM



* Diameter **Ø4.5**

Length


7	IP4507SM
8	IP4508SM
10	IP4510SM
12	IP4512SM
14	IP4514SM



* Diameter **Ø5.0**

Length


7	IP5007SM
8	IP5008SM
10	IP5010SM
12	IP5012SM
14	IP5014SM



* Diameter **Ø6.0**

Length

7	IP6007SM
8	IP6008SM
10	IP6010SM
12	IP6012SM
14	-





No-Mount Cuff 2.4mm fixture > Packing unit: 1 Fixture + 1 Cover Screw.

* Diameter **Ø3.5**

Length



7	-
8	IT3508SM
10	IT3510SM
12	IT3512SM
14	IT3514SM



* Diameter **Ø4.0**

Length



7	IT4007SM
8	IT4008SM
10	IT4010SM
12	IT4012SM
14	IT4014SM



* Diameter **Ø4.5**

Length


7	IT4507SM
8	IT4508SM
10	IT4510SM
12	IT4512SM
14	IT4514SM



* Diameter **Ø5.0**

Length


7	IT5007SM
8	IT5008SM
10	IT5010SM
12	IT5012SM
14	IT5014SM



* Diameter **Ø6.0**

Length

7	IT6007SM
8	IT6008SM
10	IT6010SM
12	IT6012SM
14	-




Cover Screw



Platform [Fixture Dia.]	Ø4.8 [Ø3.5 / Ø4.0 / Ø4.5]	Ø5.9 [Ø5.0 / Ø6.0]
Diameter	Ø5.0	
Height	Ø6.0	
6.5	ICVR002	ICVW002

- > Packing unit: 1 Cover Screw.
- > To seal the conical interface of the fixture.
- > Tightened with the 1.2 Hex Driver.
- > Tightening torque force: 5~10N.cm.


Headless Screw



Diameter	Ø3.5
Height	6
	ICVR001

- > Packing unit: 1 Headless Screw.
- > For narrow mesiodistal distance.
- > Tightened with the 1.2 Hex Driver.
- > Tightening torque force: 5~10N.cm.

Healing Abutment




Platform [Fixture Dia.]	Ø4.8 [Ø3.5 / Ø4.0 / Ø4.5]	Ø5.9 [Ø5.0 / Ø6.0]
Diameter	Ø5.5	Ø6.6
Length		
2	IHCR020	IHCW020
3	IHCR030	IHCW030
4.5	IHCR045	IHCW045


- > Packing unit: 1 Healing Abutment.
- > For remodeling gingival contour during soft tissue healing.
- > Select the abutment according to gingival height and abutment type.
- > Tightened with the 1.2 Hex Driver.
- > Tightening torque force: 5~10N.cm.

Prosthetic Procedure I

Component Selection Guide for Cemented & UCLA Abutment



Cemented Extension Abutment



Type	Octa			
Platform [Fixture Dia.]	Ø4.8 [Ø3.5 / Ø4.0 / Ø4.5]		Ø5.9 [Ø5.0 / Ø6.0]	
Diameter	Ø4.8	Ø5.8	Ø5.9	Ø6.9
Cuff Length	6	6	6	6


	0.5	IECW506	
1		IECR416	IECW516
2		IECR426	IECW526
3		IECR436	IECW536

Type	N-Octa			
Platform [Fixture Dia.]	Ø4.8 [Ø3.5 / Ø4.0 / Ø4.5]		Ø5.9 [Ø5.0 / Ø6.0]	
Diameter	Ø4.8	Ø5.8	Ø5.9	Ø6.9
Cuff Length	6	6	6	6

	0.5	IENW506	
1		IENR416	IENW516
2		IENR426	IENW526
3		IENR436	IENW536

- > Packing unit: 1 Cemented Extension Abutment + 1 Abutment Screw.
- > For Cement Retained or Screw-Cement Retained Prosthesis.
- > Cutting surface for anti-rotation of the prosthesis.
- > Connected with the Abutment Screw (ISHR110).
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 30N.cm.
- > Fixture level impression.


Angulated Abutment



Type	Octa	
Platform [Fixture Dia.]	Ø4.8 & Ø5.9 [Ø3.5 / Ø4.0 / Ø4.5 / Ø5.0 / Ø6.0]	
Diameter (Angle)	3.8 (15°)	3.8 (25°)
Length	8	8

- > Packing unit: 1 Angulated Abutment + 1 Abutment Screw.
- > For Cement Retained or Screw-Cement Retained Prosthesis.
- > Solution for the anterior esthetic zone.
- > Connected with the Abutment Screw (ISHR100).
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 30N.cm.
- > Fixture level impression.


Meta G UCLA Abutment



Type	Octa		N-Octa	
Platform [Fixture Dia.]	Ø4.8 [Ø3.5 / Ø4.0 / Ø4.5]	Ø5.9 [Ø5.0 / Ø6.0]	Ø4.8 [Ø3.5 / Ø4.0 / Ø4.5]	Ø5.9 [Ø5.0 / Ø6.0]
Diameter	Ø5	Ø6	Ø5	Ø6
Length	12	12	12	12

- > Packing unit: 1 Meta G UCLA Abutment + 1 Abutment Screw.
- > For Screw-Cement or Screw Retained Prosthesis.
- > Modification to the angulated abutment, customized abutment and telescopic abutment.
- > CCM alloy core for precise connection.
- > Cast with non-precious metal or gold alloy.
- > Connected with the Abutment Screw (ISHR120).
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 30N.cm.
- > Fixture level impression.


Abutment Screw



Diameter	Ø2.5	Ø2.5	Ø2.5
Height	6.3	ISHR100	
	7.8		ISHR120
	9.2	ISHR110	

- > Packing unit: 1 Abutment Screw.
- > ISHR110: Cemented Abutment.
- > ISHR100: Angulated Abutment.
- > ISHR120: Meta G UCLA Abutment.
- > Tightened with the 1.2 Hex Driver and Torque Wrench.


Replica



Platform [Fixture Dia.]	Ø4.8 [Ø3.5 / Ø4.0 / Ø4.5]	Ø5.9 [Ø5.0 / Ø6.0]
Diameter	Ø4.8	Ø5.9
Height	12	12
	IROR001	IROW001

- > Packing unit: 1 Replica.
- > Mimicking of the conical interface of the fixture.
- > Analog of fixture for the working cast.


Pick-up Impression Coping



Type	Octa	
Platform [Fixture Dia.]	Ø4.8 [Ø3.5 / Ø4.0 / Ø4.5]	Ø5.9 [Ø5.0 / Ø6.0]
Diameter	Ø5.5	Ø6.6
Length	13.7	13.7
	IIOR001	ILOW001

- > Packing unit: 1 Pick-up Impression Coping + 1 Guide Pin.
- > For open tray impression.
- > Connected with the Guide Pin (IIOR001S).
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 12~15N.cm.

Transfer Post




Type	Octa		N-Octa	
Platform [Fixture Dia.]	Ø4.8 [Ø3.5 / Ø4.0 / Ø4.5]	Ø5.9 [Ø5.0 / Ø6.0]	Ø4.8 [Ø3.5 / Ø4.0 / Ø4.5]	Ø5.9 [Ø5.0 / Ø6.0]
Diameter	Ø4.85	Ø5.95	Ø4.85	Ø5.95
Length	11.6	11.6	11.6	11.6
	ITOR400	ITOW500	ITNR400	ITNW500

- > Packing unit: Octa - 1 Transfer Post + 1 Guide Pin / N-Octa - 1 Transfer Post (Solid Type).
- > For closed tray impression.
- > Connected with the Guide Pin (Regular: ITOR400S / Wide: ITOW500S).
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 12~15N.cm.

Prosthetic Procedure II

Component Selection Guide for Solid Abutment

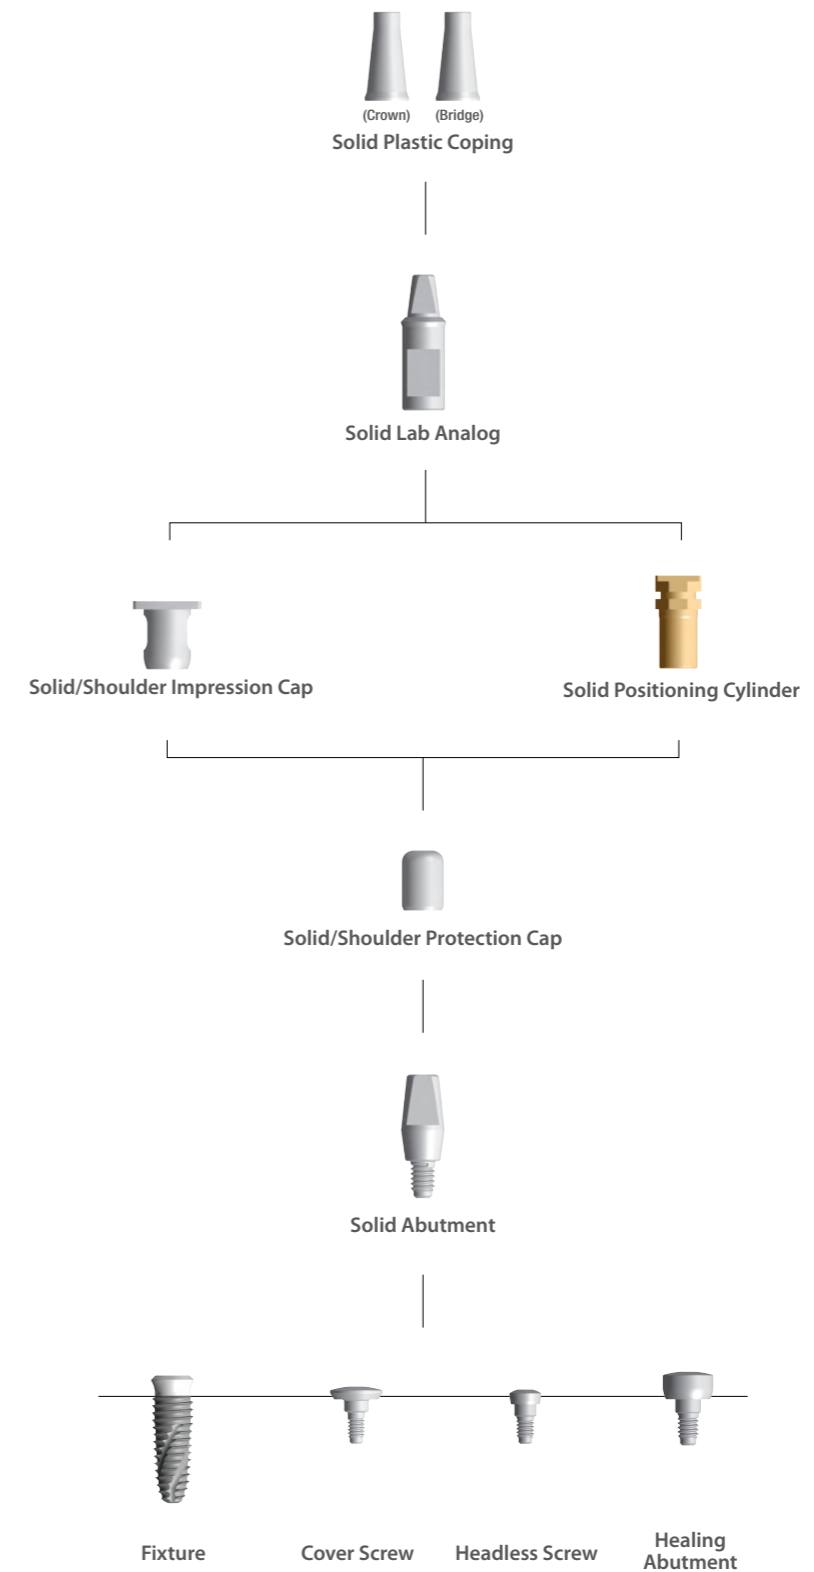


Solid Abutment



Platform [Fixture Dia.]	Ø4.8 & Ø5.9 [Ø3.5 / Ø4.0 / Ø4.5 / Ø5.0 / Ø6.0]			
Diameter	Ø3.5			
Length	3	4	5.5	7
	IASR030	IASR040	IASR055	IASR070

- > Packing unit: 1 Solid Abutment + 1 Protection Cap.
- > For Cement Retained Prosthesis.
- > Cutting surface for anti-rotation of the prosthesis.
- > Integrated with screw and abutment.
- > Tightened with the Shoulder Driver.
- > Tightening torque force: 30N.cm.
- > Abutment level impression:
Impression cap in platform Ø4.1 fixture and direct impression in platform Ø5.8 fixture.




Solid Positioning Cylinder



Solid Abutment Diameter	Ø3.5
Diameter	Ø5.7
Height	10.2
	IPCR001

- > Packing unit: 1 Solid Positioning Cylinder.
- > Inner cutting surface for anti-rotation on the abutment.
- > Insert into the Impression Cap.

Solid/Shoulder Protection Cap



Solid Abutment Diameter	Ø3.5	
Diameter	Ø5.4	
Height	5.2	IASR130
	6.2	IASR140
	7.7	IASR155
	9.2	IASR170

- > Packing unit: 1 Solid/Shoulder Protection Cap.
- > Protection from cheek and tongue for gingival healing period.
- > Alternative usage for sub-structure of the temporary prosthesis.


Solid Lab Analog



Solid Abutment Diameter	Ø3.5			
Diameter	Ø4.8			
Length	3	4	5.5	7
	ILSR030	ILSR040	ILSR055	ILSR070

- > Packing unit: 1 Solid Lab Analog.
- > Replacement of abutment shape in working cast.
- > Choose according to length of the abutment.


Solid/Shoulder Impression Cap



Solid Abutment Diameter	Ø3.5
Diameter	8
Height	8
	IICR001

- > Packing unit: 1 Solid/Shoulder Impression Cap.
- > Connected with the Solid Positioning Cylinder.
- > Confirm locking with abutment by rotation of clockwise and anti-clockwise direction.

Solid Plastic Coping




Type	Crown	Bridge
Solid Abutment Diameter	Ø3.5	Ø3.5
Diameter	Ø5	Ø5
Height	10	10
	IPCC001	IPCB001


- > Packing unit: 1 Solid Plastic Coping.
- > Connect with the Lab Analog.
- > Burn out and casting for the metal framework.

Prosthetic Procedure III

Component Selection Guide for Shoulder Abutment

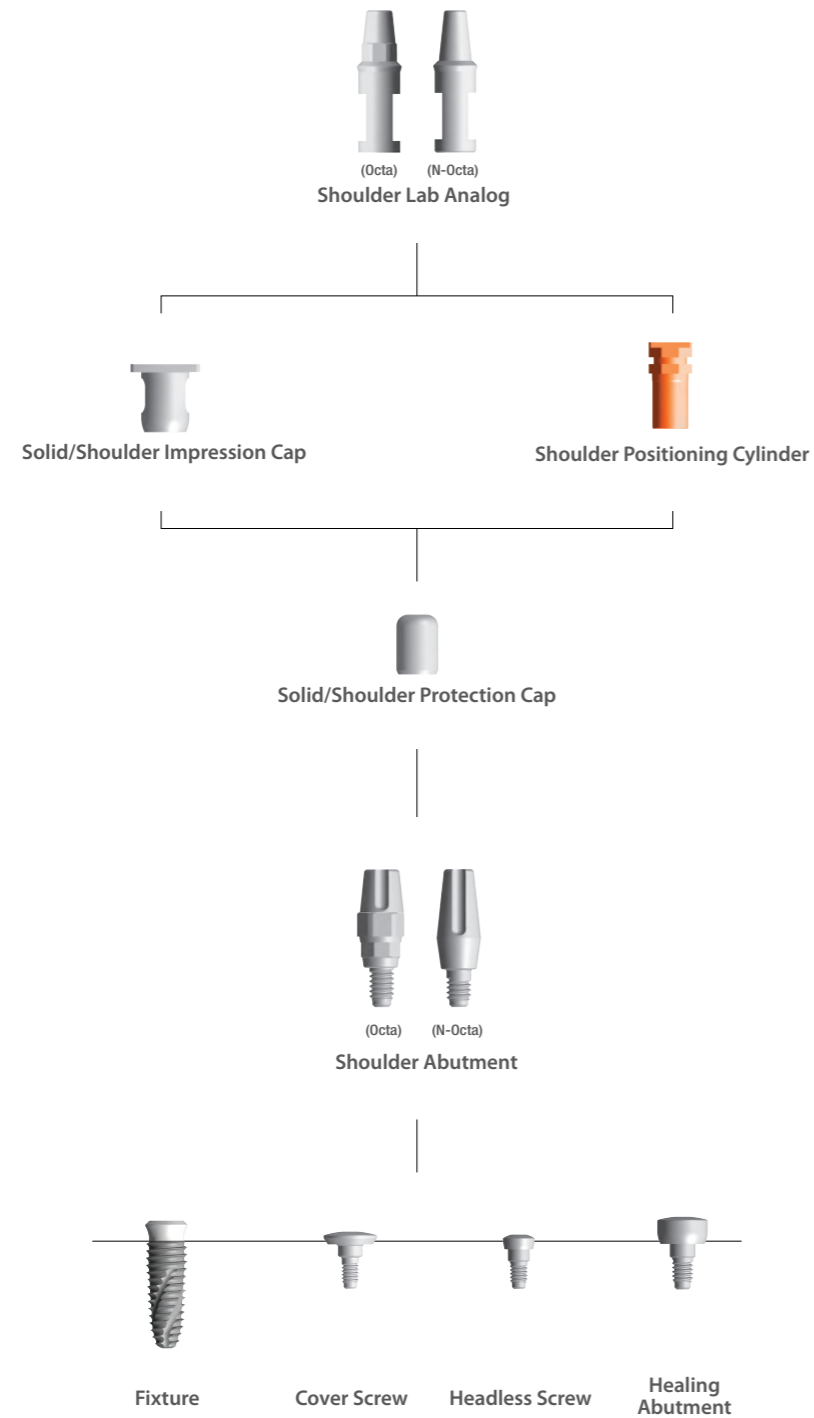

Shoulder Abutment




Type	Octa		N-Octa	
* Platform [Fixture Dia.]	Ø4.8 [Ø3.5 / Ø4.0 / Ø4.5]	Ø5.9 [Ø5.0 / Ø6.0]	Ø4.8 [Ø3.5 / Ø4.0 / Ø4.5]	Ø5.9 [Ø5.0 / Ø6.0]
Diameter	Ø3.5	Ø4.5	Ø3.5	Ø4.5
Length				
4	ISAC404	ISAC504	ISAB404	ISAB504
5.5	ISAC405	ISAC505	ISAB405	ISAB505
7	ISAC407	ISAC507	ISAB407	ISAB507

- > Packing unit: 1 Shoulder Abutment + 1 Protection Cap.
- > For Cement Retained Prosthesis.
- > Dual anti-rotation grip with a single crown for prevention of screw loosening.
- > Integrated with the Screw and Abutment.
- > Tightened with the Shoulder Driver.
- > Tightening torque force: 30N.cm.
- > Abutment level impression.




Solid/Shoulder Protection Cap



Shoulder Abutment Diameter	Ø3.5	Ø4.5
Diameter	Ø5.4	Ø5.4
Height		
6.2	IASR140	IASW140
7.7	IASR155	IASW155
9.2	IASR170	IASW170

- > Packing unit: 1 Solid/Shoulder Protection Cap.
- > Protection from cheek and tongue for gingival healing period.
- > Alternative usage for sub-structure of the temporary prosthesis.


Solid/Shoulder Impression Cap



Shoulder Abutment Diameter	Ø3.5	Ø4.5
Diameter	8	9
Height		
8	IICR001	IICW001

- > Packing unit: 1 Solid/Shoulder Impression Cap.
- > Connected with the Shoulder Positioning Cylinder.
- > Confirm locking with abutment by rotation of clockwise and anti-clockwise direction.


Shoulder Positioning Cylinder



Shoulder Abutment Diameter	Ø3.5	Ø4.5
Diameter	5.7	6.8
Height		
10.7	SAPR001	SAPW001

- > Packing unit: 1 Shoulder Positioning Cylinder.
- > Inner cutting surface for anti-rotation on the abutment.
- > Insert into the Impression Cap.

Shoulder Lab Analog




Type	Octa		N-Octa	
Shoulder Abutment Diameter	Ø3.5	Ø4.5	Ø3.5	Ø4.5
Diameter	Ø4.8	Ø5.9	Ø4.8	Ø5.9
Length				
4	SLCR040	SLCW040	SLBR040	SLBW040
5.5	SLCR055	SLCW055	SLBR055	SLBW055
7	SLCR070	SLCW070	SLBR070	SLBW070


- > Packing unit: 1 Shoulder Lab Analog.
- > Replacement of abutment shape in working cast.
- > Choose according to width and length of the abutment.

Prosthetic Procedure IV

Component Selection Guide for Sonator S&A Abutment

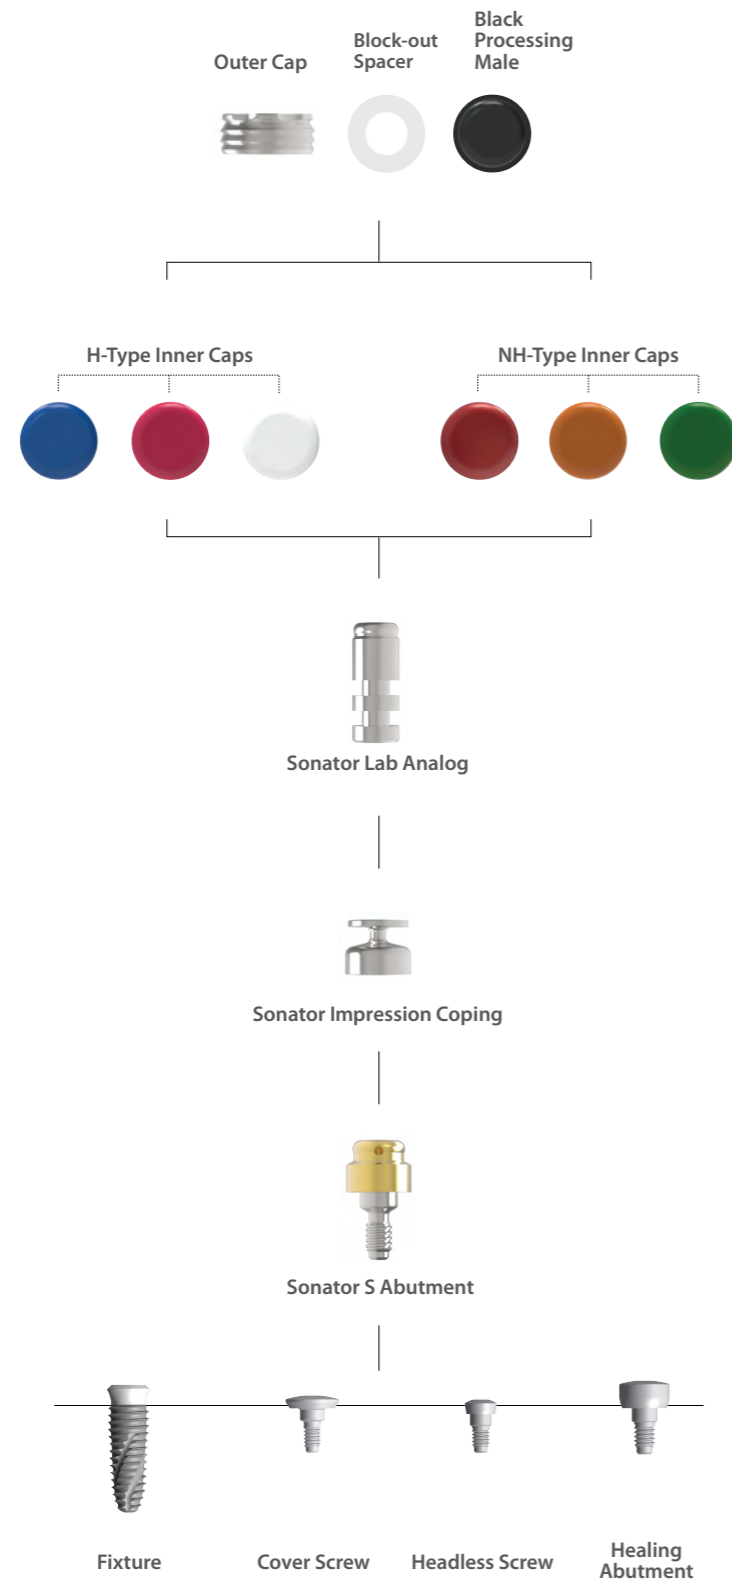

Sonator S Abutment



Diameter	Ø4.0			
Cuff Length	0.6	2	3	4
	IONS401	IONS402	IONS403	IONS404

- > Packing unit: 1 Sonator S Abutment + 1 Carrier + 3 H-Type Inner Caps + 1 Outer Cap + 1 Block-out Spacer + 1 Black Processing Male.
- > For Implant-Supported Overdenture Prosthesis.
- > Stable with low vertical height.
- > 6 kinds of Inner Caps give various holding force (Both, H and NH-Type Inner Caps are used for the Sonator S Abutment).
- > Path compensation up to 20° based on 2 implants.
- > Carrier: Used for delivery of the abutment.
- > Tightened with the Ratchet Driver and Torque wrench.
- > Tightening torque force: 30N.cm.
- > Abutment level impression.


Outer Cap



Diameter / Height	Ø5.4
2.25	SONOC01

- > Packing unit: 2 Outer Caps and 2 Black Processing Males.
- > Black Processing Male: Inserted and Removed with the I&R Driver.


H-Type Inner Cap



Code	SONIC01
------	---------


- > Packing unit: 3 Block-out Spacers + 3 Inner Caps (1 Blue, 1 Pink, and 1 White).
- > Path compensation up to 20° based on 2 implants.
- > Mainly used for the Sonator S Abutment.
- > Inner Caps: Inserted and Removed with the I&R Driver.

NH-Type Inner Cap

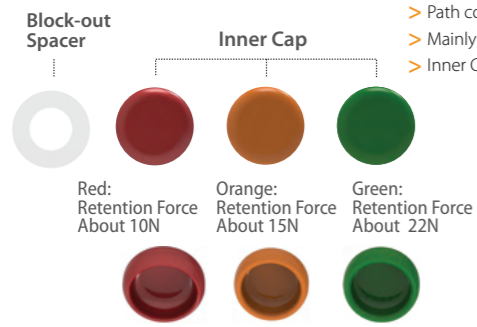

Code	SONIC02
<ul style="list-style-type: none"> > Packing unit: 3 Block-out Spacers + 3 Inner Caps (1 Red, 1 Orange, and 1 Green). > Path compensation up to 40° based on 2 implants. > Mainly used for the Sonator A Abutment. > Inner Caps: Inserted and Removed with the I&R Driver. 	


Sonator Impression Coping



Diameter	Ø4.8
Length	3
SONIP04	

- > Packing unit: 4 Impression Copings and 4 Black Processing Males.
- > Abutment level pick-up impression.
- > Connected over the Sonator Abutment after placing the Block-out Spacer.
- > For close tray impression.


Sonator Lab Analog



Diameter	Ø4
Length	1.4
SONLA04	

- > Packing unit: 4 Sonator Lab Analogs.
- > Replacement of abutment shape in working cast.


Sonator S Ratchet Driver



Type	Ratchet
Height	18
SONRD19L	

- > Packing unit: 1 Sonator S Ratchet Driver.
- > To install and remove the Sonator S Abutment with the Torque Wrench.

Sonator I&R Driver




Height	95.4
SONIR002	


- > Packing unit: 1 Sonator I&R Driver.
- > Used to insert and remove the Inner Caps and Block Processing Male.

Prosthetic Procedure V

Component Selection Guide for Ball Abutment




Ball Abutment



Diameter	Ø3.5
Length	4
IBAT404R	

- > Packing unit: 1 Ball Abutment + 3 Inner Caps (1 per each color) + 1 Block-out Spacer + 1 Outer Cap.
- > For Implant-Supported Overdenture Prosthesis.
- > Tightened with the Ball Driver and Torque Wrench.
- > Tightening torque force: 30N.cm.
- > Direct impression.


Ball Outer Cap



Diameter	Ø3.4
Height	2.4
BATC003C	

- > Packing unit: 2 Outer Caps.

Ball Inner Cap



BATC003I	
----------	--

- > Packing unit: 2 Block-out Spacers + 6 Inner Caps (2 per each color).
- > Retention force: Red 10N, Orange 15N & Green 20N.



Ball Analog



Diameter	Ø4.0
Length	4
SBAL400	

- > Packing unit: 4 Lab Analogs.
- > Replacement of abutment shape in working cast.

Ball Driver




Height	19
Type	Ratchet
KRB19L	

- > Packing unit: 1 Ball Driver.
- > To install and remove the Ball Abutment with the Torque Wrench.

*Extra Product

Ball I&R Driver












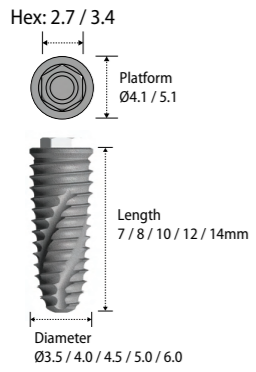




Height	100
KBIR01	

- > Packing unit: 1 Ball I&R Driver.
- > Used to insert and remove the Inner Caps into and out of the Outer Cap.

INNO EXTERNAL IMPLANT (Ext.)

System Flow


Fixture	Abutment	Impression
	<p>Prosthetic Procedure I</p> <div style="display: flex; justify-content: space-around;"> <div style="text-align: center;"> <p>102p</p>  <p>Cemented Abutment</p> </div> <div style="text-align: center;"> <p>102p</p>  <p>Angulated Abutment</p> </div> </div> <div style="display: flex; justify-content: space-around; margin-top: 10px;"> <div style="text-align: center;"> <p>102p</p>  <p>Temporary Abutment</p> </div> <div style="text-align: center;"> <p>103p</p>  <p>Meta G UCLA Abutment</p> </div> <div style="text-align: center;"> <p>103p</p>  <p>Plastic UCLA Abutment</p> </div> </div>	<p>Fixture Level Impression</p> <div style="display: flex; justify-content: space-around; margin-top: 20px;"> <div style="text-align: center;"> <p>104p</p>  <p>Replica</p> </div> <div style="text-align: center;"> <p>104p</p>  <p>Pick-up Squared Impression Coping</p> </div> <div style="text-align: center;"> <p>104p</p>  <p>Transfer Post</p> </div> </div>
	<p>Prosthetic Procedure II</p> <div style="text-align: center; margin-top: 20px;"> <p>106p</p>  <p>Shoulder Abutment</p> </div>	<p>Abutment Level Impression</p> <div style="display: flex; justify-content: space-around; margin-top: 20px;"> <div style="text-align: center;"> <p>106p</p>  <p>Solid/Shoulder Protection Cap</p> </div> <div style="text-align: center;"> <p>107p</p>  <p>Solid/Shoulder Impression Cap</p> </div> <div style="text-align: center;"> <p>107p</p>  <p>Shoulder Positioning Cylinder</p> </div> <div style="text-align: center;"> <p>107p</p>  <p>Shoulder Lab Analog</p> </div> </div>
	<p>Prosthetic Procedure III</p> <div style="text-align: center; margin-top: 20px;"> <p>109p</p>  <p>Ball Abutment</p> </div>	<p>Abutment Level Impression</p> <div style="text-align: center; margin-top: 20px;"> <p>109p</p>  <p>Ball Analog</p> </div>

INNO External Implant (Ext.)



External Fixture
Surface Treatment: **SLA-SH™**

- > Interchangeable with external hexagonal fixture.
- > External hex connection (Hex 2.7 / 3.4).



INNO Fixture Code

E	T	40	10	S	<input type="checkbox"/>
Type External	body Taper	Diameter Ø 4.0	Length 10 mm	Surface Treatment SLA	Mount Pre-Mount


*Ex.)
SLA Pre-Mount ET4010S

Pre-Mount > Packing unit: 1 Fixture + 1 Mount + 1 Mount Screw.

* Diameter **Ø3.5**

Length


7	-
8	ET3508S
10	ET3510S
12	ET3512S
14	ET3514S



* Diameter **Ø4.0**

Length


7	ET4007S
8	ET4008S
10	ET4010S
12	ET4012S
14	ET4014S



* Diameter **Ø4.5**

Length


7	ET4507S
8	ET4508S
10	ET4510S
12	ET4512S
14	ET4514S



* Diameter **Ø5.0**

Length


7	ET5007S
8	ET5008S
10	ET5010S
12	ET5012S
14	ET5014S




* Diameter **Ø6.0**

Length

7	ET6007S
8	ET6008S
10	ET6010S
12	ET6012S
14	-




Fixture Mount



Hex	Hex2.7	Hex3.4
Platform [Fixture Dia.]	Ø4.1 [Ø3.5 / Ø4.0 / Ø4.5]	Ø5.1 [Ø5.0 / Ø6.0]
Diameter	Ø4.9	Ø5.5
Length	7.2	MER001
		MEW002

- > Packing unit: 1 Mount + 1 Mount Screw.
- > Tightened with the 1.2 Hex Driver.
- > Tightening torque force: 5~10N.cm.


Cover Screw



Hex	Hex2.7	Hex3.4
Platform [Fixture Dia.]	Ø4.1 [Ø3.5 / Ø4.0 / Ø4.5]	Ø5.1 [Ø5.0 / Ø6.0]
Diameter	Ø4.3	Ø5.4
Height	5.8	VNR001
		VNW001

- > Packing unit: 1 Cover Screw.
- > To seal the conical interface of the fixture.
- > Tightened with the 1.2 Hex Driver.
- > Tightening torque force: 5~10N.cm.

Healing Abutment




Hex	Hex2.7	Hex3.4
Platform [Fixture Dia.]	Ø4.1 [Ø3.5 / Ø4.0 / Ø4.5]	Ø5.1 [Ø5.0 / Ø6.0]
Diameter	Ø5.0	Ø6.0
Length	2.8	HNR502
	3.8	HNR503
	4.8	HNR504
	5.8	HNR505
	6.8	HNR506
	7.8	HNR507
		HNW602
		HNW603
		HNW604
		HNW605
		HNW606
		HNW607


- > Packing unit: 1 Healing Abutment.
- > For remodeling gingival contour during soft tissue healing.
- > Select the abutment according to gingival height and abutment type.
- > Tightened with the 1.2 Hex Driver.
- > Tightening torque force: 5~10N.cm.

Prosthetic Procedure I

Component Selection Guide for Cemented & UCLA Abutment

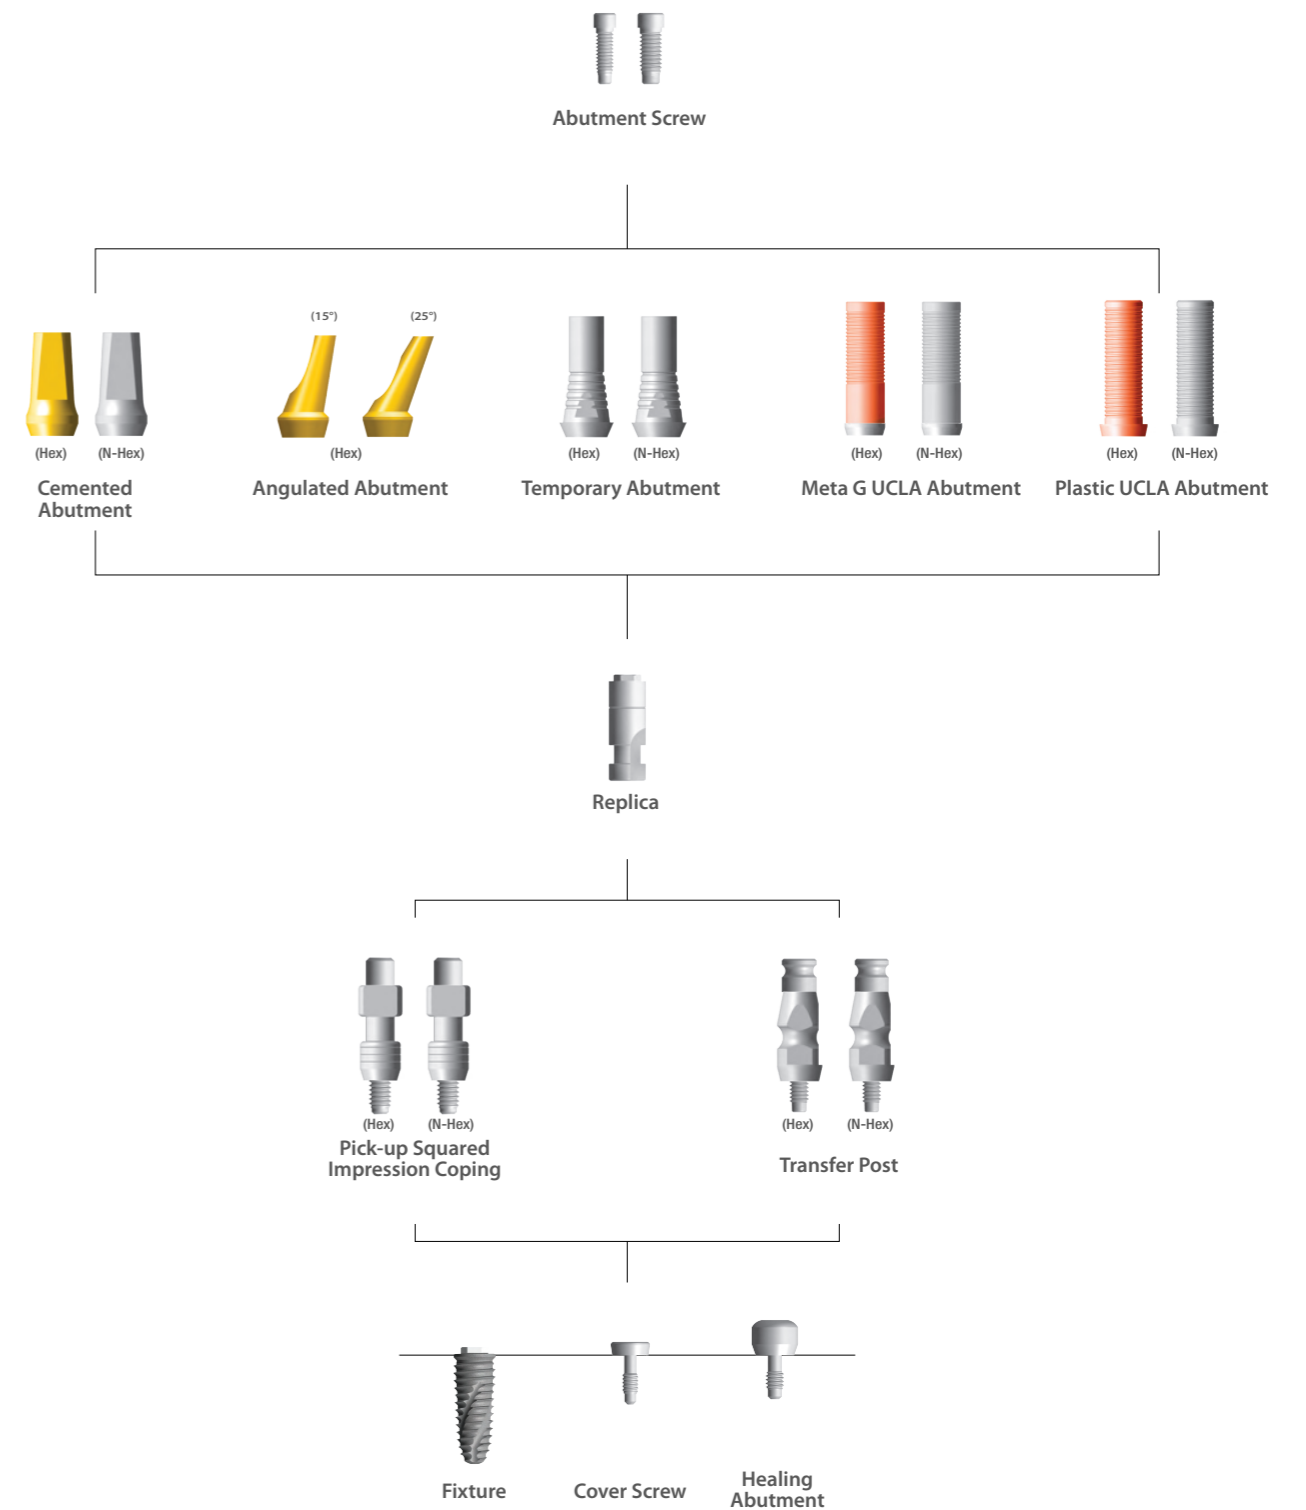

Cemented Abutment




*Type[Hex]	Hex[2.7]		Hex[3.4]	
*Platform [Fixture Dia.]	Ø4.1 [Ø3.5 / Ø4.0 / Ø4.5]		Ø5.1 [Ø5.0 / Ø6.0]	
Diameter	Ø5.0		Ø6.0	
Length Cuff	6	8	6	8
1	CHR516	CHR518	CHW616	CHW618
2	CHR526	CHR528	CHW626	CHW628
3	CHR536	CHR538	CHW636	CHW638
4	CHR546	CHR548	CHW646	CHW648

Type[Hex]	N-Hex			
Platform [Fixture Dia.]	Ø4.1 [Ø3.5 / Ø4.0 / Ø4.5]		Ø5.1 [Ø5.0 / Ø6.0]	
Diameter	Ø5.0		Ø6.0	
Length Cuff	6	8	6	8
1	CNR516	CNR518	CNW616	CNW618
2	CNR526	CNR528	CNW626	CNW628
3	CNR536	CNR538	CNW636	CNW638
4	CNR546	CNR548	CNW646	CNW648

- > Packing unit: 1 Cemented Abutment + 1 Abutment Screw.
- > For Cement Retained and Screw-Cement Retained Prosthesis.
- > Cutting surface for anti-rotation of the prosthesis.
- > Connected with the Abutment Screw.
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 30N.cm
- > Fixture level impression.


Meta G UCLA Abutment



Type[Hex]	Hex[2.7]	Hex[3.4]	N-Hex	N-Hex
Platform [Fixture Dia.]	Ø4.1 [Ø3.5 / Ø4.0 / Ø4.5]	Ø5.1 [Ø5.0 / Ø6.0]	Ø4.1 [Ø3.5 / Ø4.0 / Ø4.5]	Ø5.1 [Ø5.0 / Ø6.0]
Diameter	Ø4.5	Ø5.5	Ø4.5	Ø5.5
Length Cuff	13	13	13	13
1.2	GHR001N	GHW001N	GNR001N	GNW001N

- > Packing unit: 1 Meta G UCLA Abutment + 1 Abutment Screw.
- > For Screw-Cement or Screw Retained Prosthesis.
- > Modification to the angulated abutment, customized abutment and telescopic abutment.
- > CCM alloy core for precise connection.
- > Cast with non-precious metal or gold alloy.
- > Connected with the Abutment Screw.
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 30N.cm.
- > Fixture level impression.


Angulated Abutment



Type[Hex]	Hex[2.7]	Hex[3.4]	Hex[2.7]	Hex[3.4]
Platform [Fixture Dia.]	Ø4.1 [Ø3.5 / Ø4.0 / Ø4.5]	Ø5.1 [Ø5.0 / Ø6.0]	Ø4.1 [Ø3.5 / Ø4.0 / Ø4.5]	Ø5.1 [Ø5.0 / Ø6.0]
Diameter (Angle)	Ø5 (15°)	Ø6 (15°)	Ø5 (25°)	Ø6 (25°)
Length Cuff	8	8	8	8
2	AAR152	AAW152	AAR252	AAW252
3	AAR153	AAW153	AAR253	AAW253
4	AAR154	AAW154	AAR254	AAW254

- > Packing unit: 1 Angulated Abutment + 1 Abutment Screw.
- > For Screw-Cement or Cement Retained Prosthesis.
- > Solution for the anterior esthetic zone.
- > Connected with the Abutment Screw.
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 30N.cm.
- > Fixture level impression.


Plastic UCLA Abutment



Type[Hex]	Hex[2.7]	Hex[3.4]	N-Hex	N-Hex
Platform [Fixture Dia.]	Ø4.1 [Ø3.5 / Ø4.0 / Ø4.5]	Ø5.1 [Ø5.0 / Ø6.0]	Ø4.1 [Ø3.5 / Ø4.0 / Ø4.5]	Ø5.1 [Ø5.0 / Ø6.0]
Diameter	Ø4.5	Ø5.5	Ø4.5	Ø5.5
Length Cuff	11.8	11.8	11.8	11.8
1.2	PHR001	PHW001	PNR001	PNW001

- > Packing unit: 1 Plastic UCLA Abutment + 1 Abutment Screw.
- > Same purpose of use as Meta G UCLA Abutment but the low accuracy of connection.
- > PMMA material.
- > Connected with the Abutment Screw.
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: Finger light force during wax Pattern fabrication, 30N.cm after casting.


Temporary Abutment



Type[Hex]	Hex[2.7]	Hex[3.4]	N-Hex	N-Hex
Platform [Fixture Dia.]	Ø4.1 [Ø3.5 / Ø4.0 / Ø4.5]	Ø5.1 [Ø5.0 / Ø6.0]	Ø4.1 [Ø3.5 / Ø4.0 / Ø4.5]	Ø5.1 [Ø5.0 / Ø6.0]
Diameter	Ø5.4	Ø5.95	Ø5.4	Ø5.95
Length Cuff	12	12	12	12
1.5	THR001	THW001	TNR001	TNW001

- > Packing unit: 1 Temporary Abutment + 1 Abutment Screw.
- > For Screw-Cement Retained Prosthesis.
- > For provisional restoration.
- > Connected with the Abutment Screw.
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 20N.cm.

Abutment Screw



Type[Hex]	Hex[2.7]	Hex[3.4]
Platform [Fixture Dia.]	Ø4.1 [Ø3.5 / Ø4.0 / Ø4.5]	Ø5.1 [Ø5.0 / Ø6.0]
Diameter	Ø2.5	Ø3.0
Height	8	8
	SHR100	SHW100

- > Packing unit: 1 Abutment Screw.
- > Tightened with the 1.2 Hex Driver and Torque Wrench.


Replica



Type[Hex]	Hex[2.7]	Hex[3.4]
Platform [Fixture Dia.]	Ø4.1 [Ø3.5 / Ø4.0 / Ø4.5]	Ø5.1 [Ø5.0 / Ø6.0]
Diameter	Ø4.1	Ø5.1
Height	12	LHR001
	LHR001	LHW001

- > Packing unit: 1 Replica.
- > Mimicking of the conical interface of the fixture.
- > Analog of fixture for the working cast.


Pick-up Squared Impression Coping



Type[Hex]	Hex[2.7]	Hex[3.4]	N-Hex	N-Hex
Platform [Fixture Dia.]	Ø4.1 [Ø3.5 / Ø4.0 / Ø4.5]	Ø5.1 [Ø5.0 / Ø6.0]	Ø4.1 [Ø3.5 / Ø4.0 / Ø4.5]	Ø5.1 [Ø5.0 / Ø6.0]
Diameter	Ø5	Ø5.8	Ø5	Ø5.8
Length	17	IHR500	IHW600	INR500
	IHR500	IHW600	INR500	INW600

- > Packing unit: 1 Pick-up Squared Impression Coping + 1 Guide Pin.
- > Connected with the Guide Pin (Regular: UHR115 / Wide: UHW115).
- > For open tray impression.
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 12~15N.cm.

Transfer Post




Type[Hex]	Hex[2.7]	Hex[3.4]	N-Hex	N-Hex
Platform [Fixture Dia.]	Ø4.1 [Ø3.5 / Ø4.0 / Ø4.5]	Ø5.1 [Ø5.0 / Ø6.0]	Ø4.1 [Ø3.5 / Ø4.0 / Ø4.5]	Ø5.1 [Ø5.0 / Ø6.0]
Diameter	Ø4.8	Ø5.8	Ø4.8	Ø5.8
Length	13.1	IHR510	IHW610	INR510
	IHR510	IHW610	INR510	INW610


- > Packing unit: 1 Transfer Post + 1 Guide Pin.
- > Connected with the Guide Pin (Regular: IHR510S, IHR610S / Wide: IHW610S).
- > For closed tray impression.
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 12~15N.cm.

Prosthetic Procedure II

Component Selection Guide for Shoulder Abutment

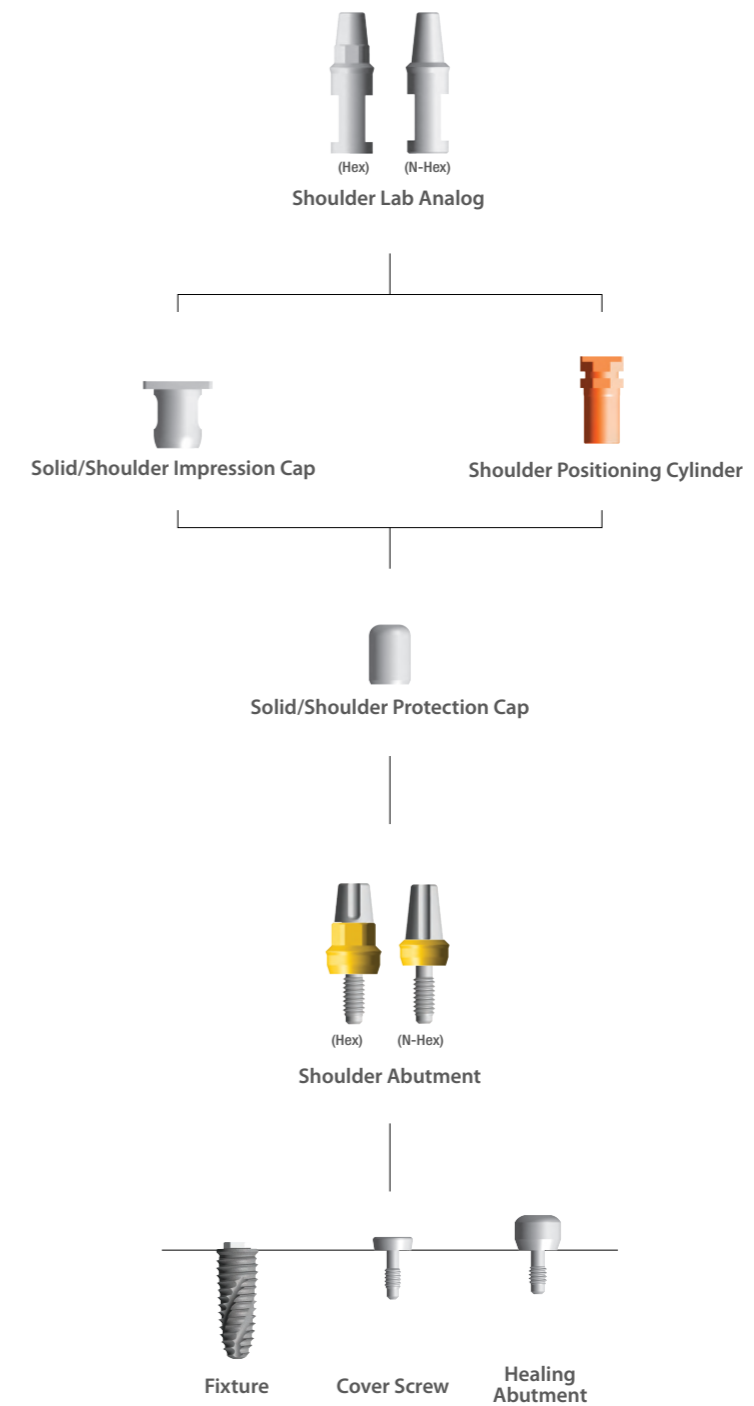


Shoulder Abutment




Type[Hex]	Hex[2.7]			Hex[3.4]		
* Platform [Fixture Dia.]	Ø4.1 [Ø3.5 / Ø4.0 / Ø4.5]			Ø5.1 [Ø5.0 / Ø6.0]		
Diameter	Ø4.8			Ø5.9		
Length Cuff	4	5.5	7	4	5.5	7
1	SAC414	SAC415	SAC417	SAC514	SAC515	SAC517
2	SAC424	SAC425	SAC427	SAC524	SAC525	SAC527
3	SAC434	SAC435	SAC437	SAC534	SAC535	SAC537
4	SAC444	SAC445	SAC447	SAC544	SAC545	SAC547

Type[Hex]	N-Hex			N-Hex		
Platform [Fixture Dia.]	Ø4.1 [Ø3.5 / Ø4.0 / Ø4.5]			Ø5.1 [Ø5.0 / Ø6.0]		
Diameter	Ø4.8			Ø5.9		
Length Cuff	4	5.5	7	4	5.5	7
1	SAB414	SAB415	SAB417	SAB514	SAB515	SAB517
2	SAB424	SAB425	SAB427	SAB524	SAB525	SAB527
3	SAB434	SAB435	SAB437	SAB534	SAB535	SAB537
4	SAB444	SAB445	SAB447	SAB544	SAB545	SAB547

- > Packing unit: 1 Shoulder Abutment.
- > For Cement Retained Prosthesis.
- > Dual anti-rotation grip with a single crown for prevention of screw loosening.
- > Integrated with screw and abutment.
- > Tightened with the Shoulder Driver.
- > Tightening torque force: 30N.cm.
- > Abutment level impression: Impression cap in platform Ø4.1 fixture and direct impression in platform Ø5.8 fixture.




Solid/Shoulder Impression Cap



Shoulder Abutment Diameter	Ø4.8	Ø5.9
Diameter	8	9
Height	IICR001	IICW001

- > Packing unit: 1 Solid/Shoulder Impression Cap.
- > Connected with the Shoulder Positioning Cylinder.
- > Confirm locking with abutment by rotation of clockwise and anti-clockwise direction.


Shoulder Positioning Cylinder



Shoulder Abutment Diameter	Ø4.8	Ø5.9
Diameter	Ø4.4	Ø5.5
Height	10.7	SAPR001
		SAPW001

- > Packing unit: 1 Shoulder Positioning Cylinder.
- > Inner cutting surface for anti-rotation on the abutment.
- > Insert into the Impression Cap.


Solid/Shoulder Protection Cap



Shoulder Abutment Diameter	Ø4.8	Ø5.9
Diameter	Ø5.4	Ø6.5
Height	6.2	IASW140
	IASR140	IASW155
	IASR155	IASW170
	IASR170	IASW170

- > Packing unit: 1 Solid/Shoulder Protection Cap.
- > Protection from cheek and tongue for gingival healing period.
- > Alternative usage for sub-structure of the temporary prosthesis.

Shoulder Lab Analog




Type[Hex]	Hex[2.7&3.4]		N-Hex	
Shoulder Abutment Diameter	Ø4.8	Ø5.9	Ø4.8	Ø5.9
Diameter	Ø4.8	Ø5.9	Ø4.8	Ø5.9
Length	4	SLCR040	SLBR040	SLBW040
	5.5	SLCR055	SLBR055	SLBW055
	7	SLCR070	SLBR070	SLBW070


- > Packing unit: 1 Shoulder Lab Analog.
- > Replacement of abutment shape in working cast.
- > Choose according to width and length of the abutment.

Prosthetic Procedure III

Component Selection Guide for Ball Abutment

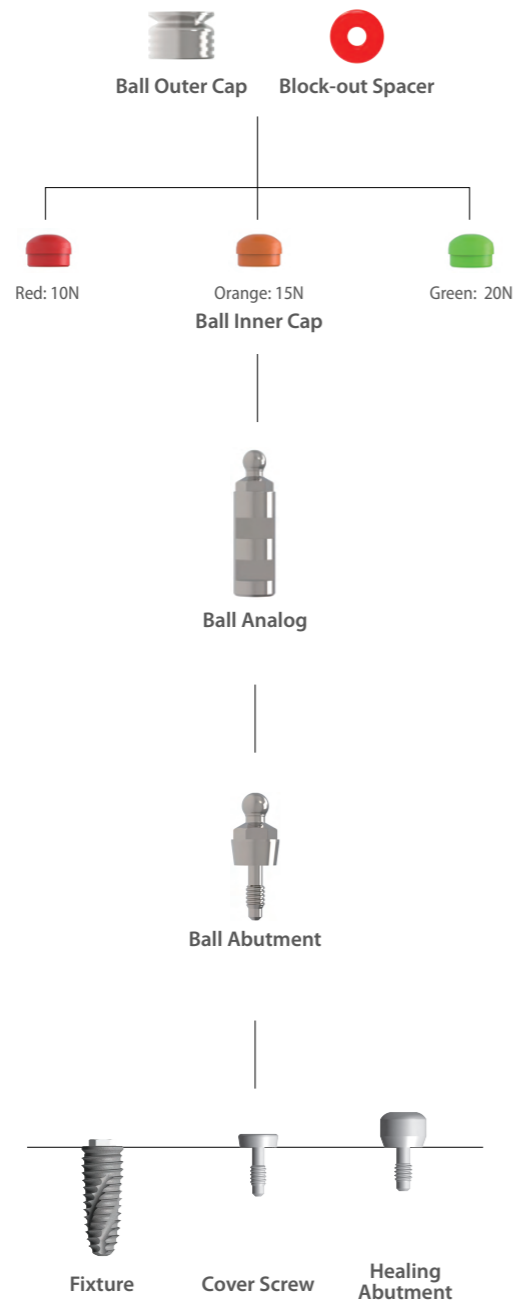


Ball Abutment



	Ø5.0	Ø6.0
Diameter	Ø5.0	Ø6.0
Length	4	4
Cuff	4	4
1	EBAT411R	EBAT511R
2	EBAT412R	EBAT512R
3	EBAT413R	EBAT513R
4	EBAT414R	EBAT514R

- > Packing unit: 1 Ball Abutment + 3 Inner Caps (1 per each color) + 1 Block-out Spacer + 1 Outer Cap.
- > For Implant-Supported Overdenture Prosthesis.
- > Tightened with the Ball Driver and Torque Wrench.
- > Tightening torque force: 30N.cm.
- > Direct impression.


Ball Outer Cap



Diameter	Ø3.4
Height	2.4
	BATC003C

- > Packing unit: 2 Outer Caps.


Ball Inner Cap



	BATC003I
	BATC003I

- > Packing unit: 2 Block-out Spacers + 6 Inner Caps (2 per each color).
- > Retention force: Red 10N, Orange 15N & Green 20N.


Ball Analog



Diameter	Ø4.0
Length	4
	SBAL400

- > Packing unit: 4 Lab Analogs.
- > Replacement of abutment shape in working cast.


Ball Driver




Type	Ratchet
Height	19
	KRB19L

- > Packing unit: 1 Ball Driver. *Extra Product
- > To install and remove the Ball Abutment with the Torque Wrench.

Ball I&R Driver



Height	100
	KBIR01



- > Packing unit: 1 Ball I&R Driver.
- > Used to insert and remove the Inner Caps into and out of the Outer Cap.

INNO SUB. FULL SURGICAL KIT [KCA010F]


SUB. HEXAGON SYSTEM

- > For INNO Submerged Implant System (Sub).
- > All components are for Sub. / Int. / Ext. except for the Fixture Drivers and the Depth Gauge used for Sub. exclusively.



Ø3.5 Fixture Final Drill
Ø4.0 Fixture Final Drill
Ø4.5 Fixture Final Drill
Ø5.0 Fixture Final Drill
Ø6.0 Fixture Final Drill

Sub. Fixture Driver							



* A common tool for Sub. / Int. / Ext. An exclusive tool by type

INNO INT. FULL SURGICAL KIT [KCA010FI]


INT. OCTAGON SYSTEM

- > For the INNO Internal Implant System (Int).
- > All components are for Sub. / Int. / Ext. except for the Fixture Drivers used for Int. exclusively.



Ø3.5 Fixture Final Drill
Ø4.0 Fixture Final Drill
Ø4.5 Fixture Final Drill
Ø5.0 Fixture Final Drill
Ø6.0 Fixture Final Drill

Int. Fixture Driver							



* A common tool for Sub. / Int. / Ext. An exclusive tool by type

INNO EXT. FULL SURGICAL KIT [KCA010FE]

EXT. HEXAGON SYSTEM

- > For the INNO External Implant System (Ext.).
- > All components are for Sub. / Int. / Ext. except for the Fixture Drivers and the Multi Countersink used for Ext. exclusively.




			* A common tool for Sub. / Int. / Ext.					An exclusive tool by type

01 Drill / Surgical Tool

SUB. HEXAGON SYSTEM
INT. OCTAGON SYSTEM
EXT. HEXAGON SYSTEM


Point Drill



- > Primarily used to mark the implant recipient site and determine the spacing.
- > The point drill has a unique pointed tip, making this an excellent drill for starting the osteotomy through the hard cortical plate.

Length	15
	KPD01S


Path Drill



- > Used for the case that path modification is required.
- > Excellent ablation force that does not slip in slanted bone.
- > Easy to drill even in extraction socket without slipping.

Length	15
	2KTD18

Initial Drill




- > Initial stepped drill - Ø2.2, Ø2.8, and Ø3.3mm stepped drilling at the Ø1.8 drilled site.

Length	8	9	11	13	15	17&19
	KPSD2207	KPSD2208	KPSD2210	KPSD2212	KPSD2214	*KPSD2218


*Extra product

Length band


- 7mm Fixture
- 8mm Fixture
- 10mm Fixture
- 12mm Fixture
- 14mm Fixture
- 16&18mm Fixture



The Initial Drill guides the pathway of the Final Drills. The Final Drill is inserted a half into the hole created by the Initial Drill without additional drilling.

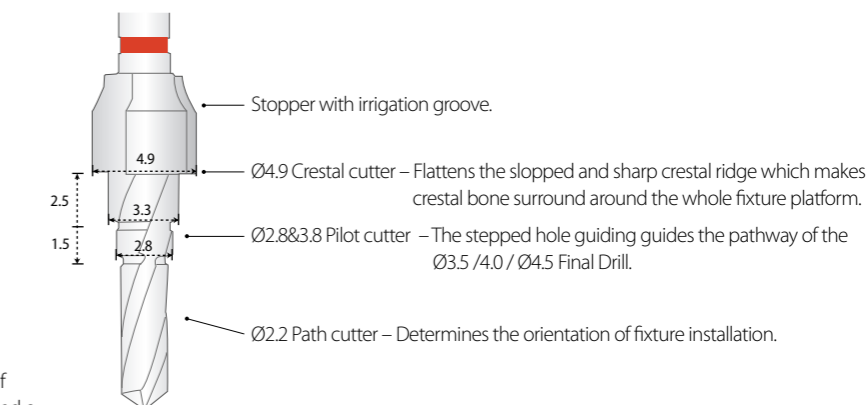

Final Drill




- > Ø3.5 / 4.0 / 4.5 / 5.0 / 6.0 fixture's Final Drill.
- > 7 / 8 / 10 / 12 / 14 / 16 / 18mm fixture's Final Drill.

Fixture Dia. Length	Ø3.5	Ø4.0	Ø4.5	Ø5.0	Ø6.0
8	2KTD3707	2KTD4007	2KTD4507	2KTD5007	2KTD6007
9	2KTD3708	2KTD4008	2KTD4508	2KTD5008	2KTD6008
11	2KTD3710	2KTD4010	2KTD4510	2KTD5010	2KTD6010
13	2KTD3712	2KTD4012	2KTD4512	2KTD5012	2KTD6012
15	2KTD3714	2KTD4014	2KTD4514	2KTD5014	
17&19	*2KTD3718	*2KTD4018	*2KTD4518		

*Extra product

Tap Drill




- > Selectively used for hard bones with bone quality 1 or higher.

Fixture Dia.	Ø3.5	Ø4.0	Ø4.5	Ø5.0	Ø6.0
	*3KMTD35A	*3KMTD40A	*3KMTD45A	*3KMTD50A	*3KMTD60A


*Extra product

Countersink




- > Used to prevent compressive necrosis of dense cortical bone by decreasing torque force (Ø4.0 Fixture: 80N.cm -> 45N.cm / Ø5.0 Fixture: 150N.cm -> 45N.cm).
- > Bone quality 1: high compressive placement of fixtures induces the failure of osseointegration and bone loss.

Fixture Dia.	Ø3.5	Ø4.0	Ø4.5	Ø5.0	Ø6.0
Diameter	Ø3.7	Ø4.2	Ø4.6	Ø5.1	Ø6.0
	4KCS35	4KCS40	4KCS45	4KCS50	4KCS60




The lower margin of the depth marking indicates exactly the level of the fixture platform.



The upper margin of the depth marking indicates 1 mm higher than the level of fixture platform.


Parallel Pin




- > Insert the Parallel Pin after the Ø2.2 or 3.5 Drill to check the drilling path.
- > In order to prevent losing Parallel Pin in the patient's mouth, be sure to tie floss through the hole in the Parallel Pin.

Height	21
	KPP002

After the Ø2.2 Initial Drill. After the Ø3.5 Final Drill.




Multi Countersink




Diameter	Ø6.5
	4KCS01

- > Only for the Ext.




Drill Extension





- > Used for lengthening the Drill when using a Hand-piece.
- > Do not go over recommended torque when using the Drill Extension.

Height	27.5
	KDE002



The triangle mark indicates the cutting surface of the drill shaft.

Mount Driver



- > Used to install Pre-Mount type fixtures.
- > The Machine Drivers are used with a contra-angle, while the Ratchet Drivers are used with the Torque Wrench.


Type	Machine
20.5(Short)	*KMMD06S
26.3(Long)	KMMD06L
32.3(X-Long)	*KMMD12X

*Extra product

Type	Ratchet
12(Short)	*KRMD12S
19(Long)	KRMD19L

*Extra product

Hex Driver




- > Used to install or remove the Cover Screw, Healing Abutment, and Abutment Screw, etc.
- > The Machine Drivers are used with contra angle, while the Ratchet Drivers are used with the Torque Wrench.

Type	Machine	
Height	Hex 0.9	Hex 1.2
22(Short)	*KMD09S	*KMD12S
28(Long)	*KMD09L	*KMD12L

*Extra product

Type	Ratchet	
Height	Hex 0.9	Hex 1.2
12(X-Short)	-	*KHD1212
17(Short)	*KHD0915	*KHD1215
23(Long)	*KHD0921	KHD1221
29(X-Long)	*KHD0927	KHD1227

*Extra product



Fixture Driver





- > Used to install No-Mount type fixtures.
- > The Machine Drivers are used with a contra-angle, while the Ratchet Drivers are used with the Torque Wrench.

Type	Machine				
Length	System	Sub.	Int.	Ext.(Hex 2.7)	Ext.(Hex 3.4)
28.1 / 26.3 / 26.4 (Short)		2KMMS01S	KMMI01S	KMME01S	KMME02S
33.3 / 30.5 / 31.4 (Long)		2KMMS01L	KMMI01L	*KMME01L	
40.3 / 35.5 / 36.4 (X-Long)		*2KMMS01X	*KMMI01X	*KMME01X	

*Extra product

Type	Ratchet				
Length	System	Sub.	Int.	Ext.(Hex 2.7)	Ext.(Hex 3.4)
20.7 / 19.5 / 19.9 (Short)		*2KHDS01S	KHDI01S	*KHDE01S	
25.7 / 24.5 / 24.9 (Long)		2KHDS01L	KHDI01L	KHDE01L	KHDE02L
30.7 / 29.5 / 29.9 (X-Long)		2KHDS01X	*KHDI01X	*KHDE01X	

*Extra product



Torque Wrench



- > Used to control torque force in the fixture and abutment placement.
- > Torque force 10, 25, 30 & 35N.cm are able to be controlled by pulling the elastic bar.
- > Maximal torque force 120N.cm with pulling the rigid main bar.

Code	KTW001
------	--------



Depth Gauge



- > Used to measure the drilling depth with the scale rod.
- > The flat end on the other side measures the 5mm space between adjacent fixtures.

Code	KDG001
------	--------




- > One side of the Depth Gauge measures the drilling depth and the other side measures the gingival height from the top of the fixture.


Code	KDG004	※ Exclusive for the Sub.
------	--------	--------------------------

02 Drilling Sequence E.g. 12mm Fixture


> Minimal drilling sequence with the Point Drill, Initial Drill and Final Drills (Ø3.5, Ø4.0 and Ø4.5 Fixtures).



> Length Marking




Actual length of the Drill: Fixture + 1mm



> Ø5.0 fixture: a series of the Point Drill, Initial Drill, Ø4.0 Final Drill, and Ø5.0 Final Drill.

> Ø6.0 fixture: a series of the Point Drill, Initial Drill, Ø4.0 Final Drill, Ø5.0 Final Drill, and Ø6.0 Final Drill.




※ The Countersink and Tap Drill should be used in hard bone quality.


*Extra product

※ Sloped edentulous ridge adjacent to tooth

> Use the crestal cutter of the Initial Drill and Final Drill.
> Longer drill than fixture's length can be used as well.




Crestal flattening



Longer Final Drill


※ Wide extraction socket

> Absence of the cortical bone & spongy bone.
> Use the drill with narrower diameter than the fixture's diameter.



※ Torque force control


> 0.5mm deeper placement increases the initial torque force of the fixture.



0.5mm deeper level.

Level	Fixture placement level					
	Crestal Level			0.5mm Deeper Level		
Density	D1	D2	D3	D1	D2	D3
Torque	34.1	29	15.5	44.4	38.4	19.1


> The pumping action while drilling removes the bone chip in the hole.
> In dense bone, the debridement removal decreases the torque force.



Density	Pumping action while final drilling		
	D1	D2	D3
Non-Debridement	34.1	29	19.6
Debridement	30	25	15.5

※ In maxillary tuberosity with bone quality 4

> No pumping action.
> 0.5mm deeper placement of the fixture.
> Wider fixture than the Final Drill.



0.5mm deeper level.

Level	Fixture placement level			
	Crestal level		0.5mm Deeper Level	
Debridement	with	without	with	without
Ø4.5 Fixture	4.4	10.2	-	12.9
Ø5.0 Fixture	11.6	19.9	14.1	24.5


INNO SUB. SMART SURGICAL KIT [KSA002]

SUB. HEXAGON SYSTEM


- > For the INNO Submerged Implant System (Sub. / Diameter: 3.5, 4.0, 4.5 & 5.0mm / Length: 8, 10, 12 & 14mm).
- > A simpler surgical kit mainly used with the Drills and Stoppers.



Length Marking & Stopper Actual length of the Drill: Fixture length + 1mm



Drilling Sequence



Point Drill	Initial Drill	Final Drill				
Point Drill KPD01S	Initial Drill 2KTD22	Ø3.5 Final Drill 2KTD35	Ø4.0 Final Drill 2KTD40	Ø4.5 Final Drill 2KTD45	Ø5.0 Final Drill 2KTD50	
Stopper			Countersink			
8 Drill Stopper KSDS08S	10 Drill Stopper KSDS10S	12 Drill Stopper KSDS12S	Ø3.5 Countersink 4KCS35	Ø4.0 Countersink 4KCS40	Ø4.5 Countersink 4KCS45	Ø5.0 Countersink 4KCS50
Drill Extension	Fixture Driver		Hex Driver			
Drill Extension KDE002	M. Fixture Driver L 2KMS01L	R. Fixture Driver L 2KHDS01L	1.2 Hex Driver L KHD1221	1.2 Hex Driver XL KHD1227	Torque Wrench KTW001	

* For Pre-Mount type of fixtures, use the Mount Drivers (*Extra product).

INNO SUB. SHORT SURGICAL KIT [KSI001]


SUB.
HEXAGON
SYSTEM

> For the INNO Submerged Short Implant System (Sub).




Length Marking & Stopper


Actual length of drill: Fixture + 0.5mm.



Drilling Sequence



Point Drill



Step Drill




Stopper



Countersink




Mount Driver



Hex Driver



Torque Wrench





INNO SUB. NARROW SURGICAL KIT [KNA001]

SUB-N.
HEXAGON
SYSTEM

> For the INNO Submerged Narrow Implant System (Sub-N).




Fixture Driver




Type	Machine	Ratchet
	KMMS01XN	KHDS01XN

- > Used to install No-Mount type fixtures.
- > The Machine Driver is used with a contra-angle, while the Ratchet Driver is used with the Torque Wrench.
- > For Pre-Mount type of fixtures, use the Mount Drivers (*Extra product).

Parallel Pin




Code	KPP003
------	--------




Point Drill	Twist Drill			
Point Drill KNPD20	Ø2.2 Twist Drill KNSD22L	Ø2.6 Twist Drill KNSD26L	Ø3.1 Twist Drill KNSD31L	Ø3.3 Twist Drill KNSD33L
Stopper	Countersink			
8 Drill Stopper KNDS08	10 Drill Stopper KNDS10	12 Drill Stopper KNDS12	Ø3.1 Countersink 4KCS31N	Ø3.3 Countersink 4KCS33N
Fixture Driver	Parallel Pin	Hex Driver	Depth Gauge	
Fixture Driver (Ratchet) KHDS01XN	Parallel Pin KPP003	1.2 Hex Driver L KHD1221	Depth Gauge KDG001	
Torque Wrench				
Torque Wrench KTW001				

Drilling Sequence




INNO PROSTHETIC PLANNING KIT [KIPP001]



- > Exclusive for the INNO Submerged and Submerged Narrow Implant System.
- > Try-in Kit for determining abutment specifications.
- > Insert the Abutment Gauge after INNO Submerged and Submerged Narrow fixture fixation to check the abutment size.




Angulated



- > Predicting Angulated Type Diameter, Cuff, and Length to help select the correct size abutment and crown.

Angulated I Beauty-up™ Abutment



Abutment Gauge



Type	Hex-A	
Diameter(Angle)	Ø4.5(15°)	Ø4.5(25°)
Cuff / Length	8	
2	P2SAH45152A	P2SAH45252A
4	P2SAH45154A	P2SAH45254A

Type	Hex-B	
Diameter(Angle)	Ø4.5(15°)	Ø4.5(25°)
Cuff / Length	8	
2	P2SAH45152B	P2SAH45252B
4	P2SAH45154B	P2SAH45254B


- > Packing unit: 1 Abutment Gauge.
- > Solution for the anterior esthetic zone.
- > Connected with the INNO Submerged Fixture.
- > Select 15° or 25° according to the case.
- > Select Hex-A or Hex-B according to the case.

Straight

- > Predicting Straight Type Diameter, Cuff, and Length to help select the correct size abutment and crown.
- Cemented | Absolute | Straight Abutment



- **Breakaway Stopper**
Prevents breakaway from intraoral cavity by connection silk.
- **Cuff Marking**
Marked Cuff 2 or 4.
- **Cuff Height**
Select Cuff 2 or 4 according to the case.
- **Diameter**
Colored by diameter.



Abutment Gauge



Type	Regular		
Diameter	Ø4.5	Ø5.5	Ø6.5
Cuff / Length	7		
2	P2SCH4527	P2SCH5527	P2SCH6527
4	P2SCH4547	P2SCH5547	P2SCH6547

- > Packing unit: 1 Abutment Gauge.
- > Solution for the straight type abutment.
- > Connected with the INNO Submerged Fixture.
- > Select Ø4.5/5.5/6.5 according to the case.

Abutment Gauge-N



Type	Narrow	
Diameter	Ø3.8	Ø4.5
Cuff / Length	7	
2	PSCH3827N	PSCH4527N
4	PSCH3847N	PSCH4547N

- > Packing unit: 1 Abutment Gauge-N.
- > Solution for the straight type abutment.
- > Connected with the INNO Submerged Narrow Fixture.
- > Select Ø3.8 or 4.5 according to the case.

Abutment Gauge-N



Type	Hex-A			
Diameter(Angle)	Ø3.8(15°)	Ø3.8(25°)	Ø4.5(15°)	Ø4.5(25°)
Cuff / Length	8			
2	PSAH38152NA	PSAH38252NA	PSAH45152NA	PSAH45252NA
4	PSAH38154NA	PSAH38254NA	PSAH45154NA	PSAH45254NA

Type	Hex-B			
Diameter(Angle)	Ø3.8(15°)	Ø3.8(25°)	Ø4.5(15°)	Ø4.5(25°)
Cuff / Length	8			
2	PSAH38152NB	PSAH38252NB	PSAH45152NB	PSAH45252NB
4	PSAH38154NB	PSAH38254NB	PSAH45154NB	PSAH45254NB

- > Packing unit: 1 Abutment Gauge-N.
- > Solution for the anterior esthetic zone.
- > Connected with the INNO Submerged Narrow Fixture.
- > Select 15° or 25° according to the case.
- > Select Hex-A or Hex-B according to the case.

INNO PROSTETIC INSTRUMENT KIT [KPA004]



> All-in-one kit for all types of the INNO Implant System (Sub. Sub-N. Int. Ext.)



1.2 Hex Driver

 12mm KHD1212	 17mm KHD1215	 23mm KHD1221	 29mm KHD1227	 39mm KHD1239	 Short KMD12S	 Long KMD12L
Ratchet				Machine		

Angulated Screw Driver

 Short KRBUD15	 Long KRBUD20
----------------------	---------------------

Multi Driver and Holder

 Ratchet KRMSD15L	 Machine KMMSD21L	 Multi S KMHS01	 Multi A KMHA01
Multi S Driver		Holder	

Straight/Solid/Shoulder Driver

 Short KRR12S	 Long KRR19L
Regular	

Lock Driver

 Short KRW12S	 Long KRW19L	 Short KRLRD18	 Long KRLRD28
Wide			

Absolute Driver

 Short KRAD4512S	 Long KRAD4519L	 Short KRAD5512S	 Long KRAD5519L	 Short KRAD6512S	 Long KRAD6519L
Ø4.5		Ø5.5		Ø6.5	

Sonator

 S Ratchet Driver SONRD19L	 I&R Driver SONIR002
----------------------------------	----------------------------

Ball

 Driver KRB19L	 I&R Driver KBIR01
----------------------	--------------------------

Torque Wrench

 Torque Wrench KTW001

Mini Plus® Implant system

Mini Plus® Implant

Cement Type


Ball Type

Surgical kit


DESIGN OF MINI PLUS® FIXTURE (1P-C.)

Cement Type

- > For mandible anterior spaces and edentulous arch.
- > For semi-permanent or temporary solution.



System Flow




Fixture

Length	Cuff	Ø2.5		Length	Cuff	Ø3.0	
		2.0mm	4.0mm			2.0mm	4.0mm
10mm		AMC2210S	AMC2410S	10mm		AMC3210S	AMC3410S
12mm		AMC2212S	AMC2412S	12mm		AMC3212S	AMC3412S
14mm		AMC2214S	AMC2414S	14mm		AMC3214S	AMC3414S

- > Packing unit: 1 Fixture.
- > Abutment level impression.

Impression Coping / Lab Analog




Impression Coping

- > Packing unit: 1 Impression Coping.
- > Used for impression taking of the post of the fixture.
- > Direct impression is recommended when modified/alterd.

Lab Analog

- > Packing unit: 1 Lab Analog.
- > The same adjustment must be made for the Lab Analog when the abutment portion of the fixture is modified/alterd.
- > Replacement of the cement post shape in working cast.

Protection Cap




Diameter	Height	Ø4.0
7mm		AMCC001
9mm		AMCC002
11mm		AMCC003

- > Packing unit: 1 Protection Cap.
- > Provides temporary protection from mucosa, gingiva, and tongue after implantation.


DESIGN OF MINI PLUS® FIXTURE (1P-B.)

Ball Type

> For semi-permanent or temporary solution for overdenture prosthesis.



System Flow



Fixture


Length	Cuff	Diameter Ø2.5	
		2.0mm	4.0mm
10mm		AMB2210S	AMB2410S
12mm		AMB2212S	AMB2412S
14mm		AMB2214S	AMB2414S

> Packing unit: 1 Fixture.

Length	Cuff	Diameter Ø2.5	
		2.0mm	4.0mm
10mm		AMB3210S	AMB3410S
12mm		AMB3212S	AMB3412S
14mm		AMB3214S	AMB3414S

> Packing unit: 1 Fixture.


Ball Outer Cap



Diameter	Height	Code
Ø3.4	2.4	BATC003C

> Packing unit: 2 Outer Caps.


Ball Inner Cap



Code
BATC003I

> Packing unit: 2 Block-out Spacers + 6 Inner Caps (2 per each color).
> Retention force: Red 10N, Orange 15N & Green 20N.

Impression Coping / Lab Analog




Impression Coping

> Packing unit: 1 Impression Coping.
> Used for impression taking of the post of the fixture.


Lab Analog

> Packing unit: 1 Lab Analog.
> Replacement of the ball post shape in working cast.


SURGICAL KIT [KMA003]




Point Drill




Ø1.3 Twist Drill



Ø1.8 Twist Drill



Ø2.3 / Ø2.6 Twist Drill



Driver



Cement Type



Ball Type




Tissue Punch *Extra product



- > Easy removal of soft tissue for flapless surgery.
- > 0.3mm wider than fixture diameter allows more predictable results.


Multi Gauge *Extra product

> Allows precise measurement of drilling depth and path.




Drilling Sequence

Ø2.5



Ø3.0



※ For bone quality 4, the Mini Plus® fixtures should be self-tapped and placed by making proper adjustments in drilling as they have self-tapping characteristics, and their diameter is narrow.

COWELL® DIGITAL PRODUCTS

Drive yourself to COWELLMEDI's Digital Transformation



Digital Guided Surgery Kit

- InnoFit Lodestar Plus Kit
- InnoFit Lodestar Kit

InnoFit Lodestar Plus Kit



Exclusive for the INNO Submerged and Submerged Narrow Implant System.

InnoFit Lodestar Kit




Universal to any implant system.

Digital Prosthesis


InnoFit Hybrid Ti-Base System

- Sub. Hybrid Ti-Base System
- Sub. & Sub-N. Multi Hybrid Ti-Base System
- Sub. Lock Hybrid Ti-Base System
- Sub-N. Hybrid Ti-Base System
- Int. Hybrid Ti-Base System




InnoFit Lodestar Plus Kit [KLSP001]

- > A total guided surgery solution applicable to various types of clinical cases.
- > Exclusive for the INNO Submerged and Submerged Narrow Implant System.



Workflow

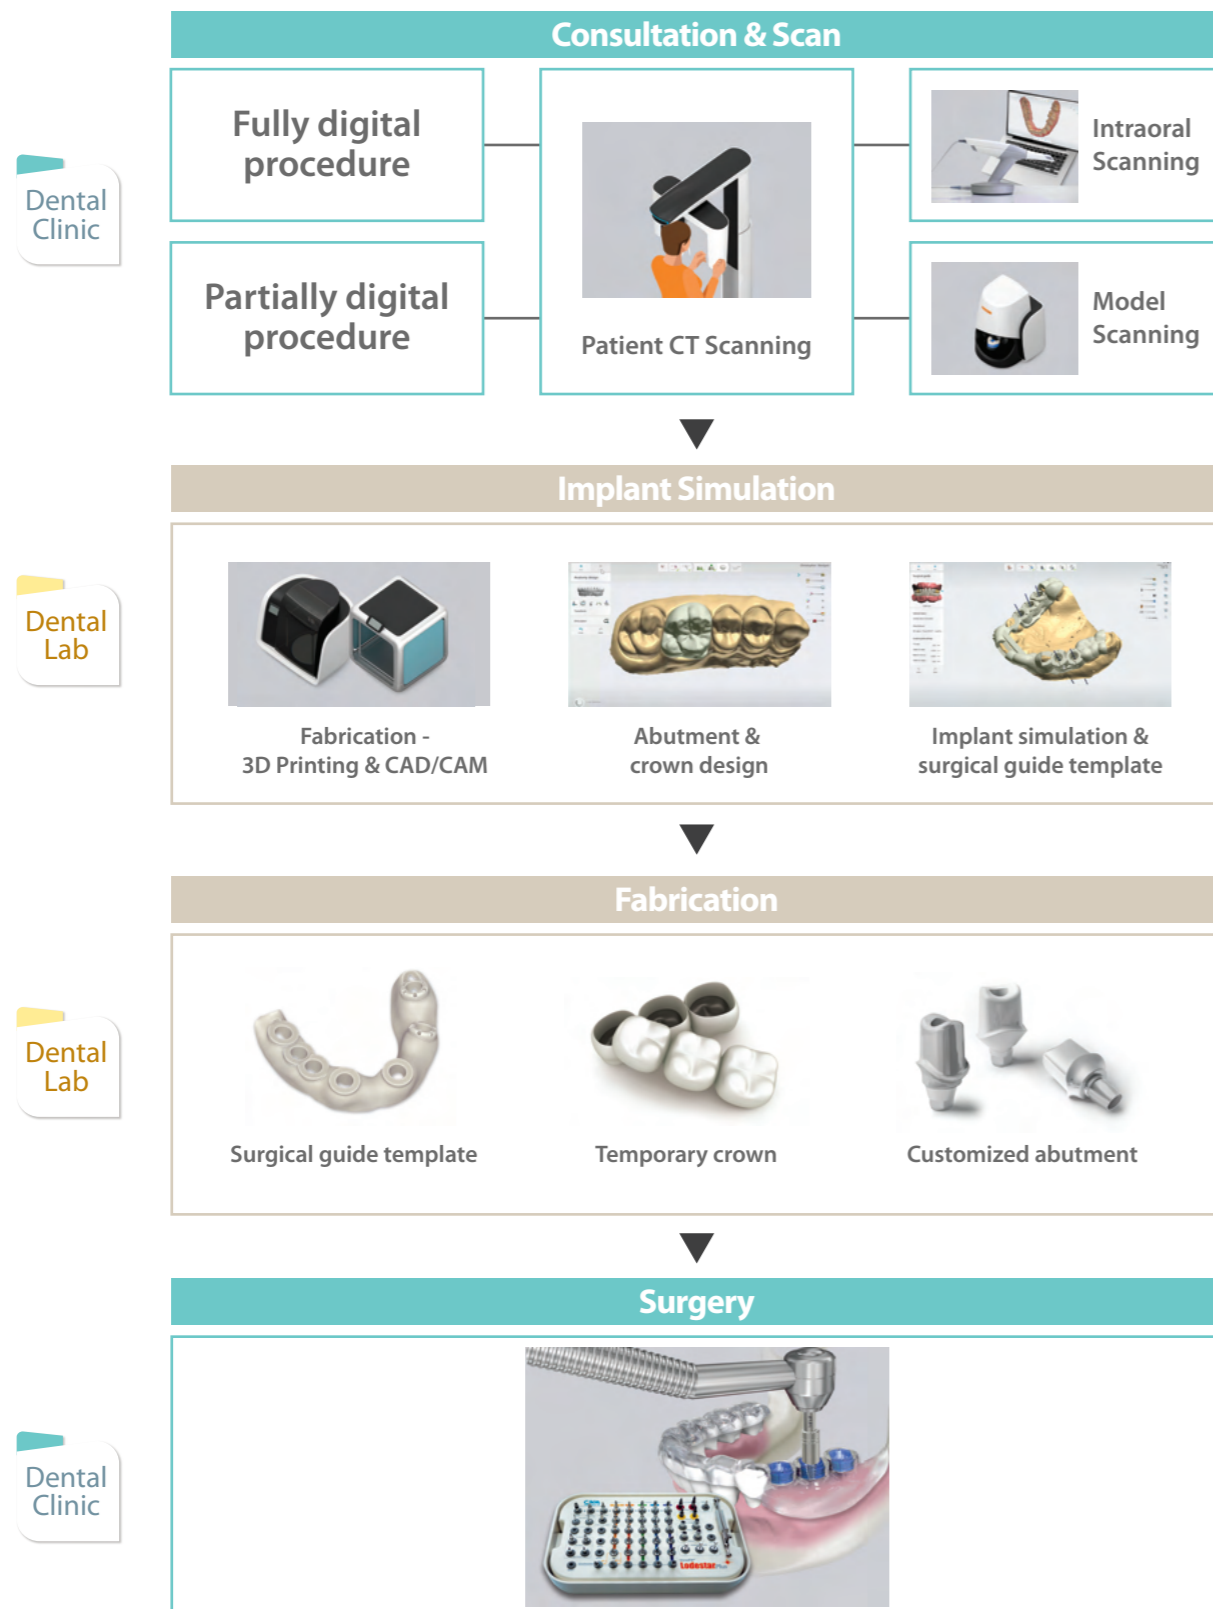

Preparation before Operation

- Disinfection of surgical guide template**




Disinfection must be done before the operation. Immerse the surgical guide template into the alcohol and chlorhexidine solution in a ratio of 9:1 or disinfection fluids such as Cidex OPA, betadine, etc. for more than 20 minutes. Then rinse with the saline solution and install in patient's oral cavity.
- Installation of surgical guide template**
 - Check if inward of the surgical guide template and outward of teeth are accurately contacted through the windows of mounted surgical guide template. In case of insufficient scan data, delete and adjust the inner side of the surgical guide template to contact precisely.
 - Install the surgical guide template while scanning CT to check implantation path and precision before the operation (Implantation path may also be checked in post operation by scanning CT with installation of the surgical guide template).
- Verification of dental implant**

Check if the marked dental implant is in the surgical report.
- Confirmation of protocol**


Confirm the surgical report and surgical protocol for the last time.

Comprehension and Usage of Offset

- > The basic length from the fixture platform to the top of the Sleeve is 9mm.
- > In case the gingiva is thick or fixture needs to be placed deeper due to low bone density, use the Sleeve 2 or 4mm upright to the top.
- > The higher the offset value, the less accurate it is, so use 9mm if possible.




Tissue Punch



- > Used for soft tissue elimination (the gingiva in the position where the implant is to be placed can be incised in a circular shape).
- > Hemostatic effect, small scar, or fast wound healing effect is occurred after the operation due to the small diameter of tissue punch.
- > Able to apply offset (9mm, 11mm, 13mm).
- > 50rpm without irrigation.

Double blade

The internal cutting edge of the Tissue Punch cuts the gingiva into small pieces so that those can be removed by suction without extra work.




*** Caution** The Tissue Punch must be kept clean. Otherwise, it may cause rust or blade damage due to residual gingival pieces or others in the Tissue Punch after the operation (remove the residual gingiva piece by explorer, steam and etc.).


Bone Flattening Drill




- > Flattens the bone level of the operation site.
- > Inclined bone level may glide the Drill and can not drill as planned.
- > Eliminates the soft tissue after using the Tissue Punch.
- > The point in the middle of the Drill guides the position of the Drill and helps to drill in an accurate site.
- > Able to apply offset (9mm, 11mm, 13mm).
- > 400rpm without irrigation / 800rpm with irrigation.



Initial Drill




- > High speed, 1,000rpm with irrigation.




Point

Creates the hole on the bone surface so that the axis of the next step Drill is not moved and it guides the Drill position by preventing slip even at the inclined bone level.


Ø3.1/Ø3.3 Fixture




Ø3.5 Fixture




Ø4.0 Fixture



Ø4.5 Fixture




Ø5.0 Fixture




Countersink

- > Expands the cortical bone in D1/D2 bone to prevent excessive implantation of the fixture.
- > Able to apply offset (9mm, 11mm, 13mm).
- > 50rpm without irrigation.




Fixture Driver - Molar

- > Used in case the Implant Adapter can not be used due to the low occlusal height.
- > After implanting 4~5mm, change to the Implant Adapter to complete the placement.




Adapter Extension

- > In case the Implant Adapter is too short to use, connect the Ratchet or Machine Adapter Extension to place the fixture.




Abutment Profiler

- > Used for the elimination of the alveolar bone that interferes with the accurate connection of abutment. Remove residual bone by rotating and drilling 360°.
- > In case of thick cortical bone, higher the drilling rpm and use with irrigation (within 100rpm).



Implant Adapter

- > Moves fixture to the Sleeve to implant safely.
- > Matches the depth of laser marks of the Sleeve offset and the Implant Adapter.
- > When implanting the fixture, the direction of the Implant Adapter and directional identification groove of the Sleeve are matched, it lines with the hex direction of the temporary abutment.
- > In case the Implant Adapter can not be removed by cold welding after placing the fixture, hang the crown remover on the groove to remove.



V Anchor - Fix Fixture


> Used with the 1.2 Hex Driver to fix the surgical guide template to the fixture in such cases as edentulous teeth.



*** Caution**
 > Install by aligning to the Sleeve offset of the placed fixture.
 > The V Anchors for the offset 11 and 13mm in length are extra products.

V Anchor - Fix Bone

> Used with the Torque Wrench to fix the surgical guide template into the hole of the bone created after initial drilling in such cases as edentulous teeth.



*** Caution**
 > Install by aligning to the Sleeve offset of the placed fixture.
 > The V Anchors for the offset 11 and 13mm in length are extra products.


1.2 Hex Ratchet Driver

> Used to install or remove the Cover Screw, and Healing Abutment.





Torque Wrench(Square)

> Used to control torque force in the fixture and abutment placement.
 > Used with the Implant Adapter, 1.2 Hex Drier, and V Anchor, etc.
 > Torque force 10, 25, 30 & 35N.cm are able to be controlled by pulling the elastic bar.
 > Maximal torque force 120N.cm with pulling the rigid main bar.




Sleeve *Extra*



Drilling Sequence


Drilling Sequence (7~10mm)

INNO Sub Fixture Ø5 x 10mm




Drilling Sequence (12~14mm)

INNO Sub Fixture Ø5 x 14mm




8~10mm drilling should be done in advance for the sleeve contact.

- * Drilling method**
- > Make sure with drilling in the desired direction without a change in the path through the primary drill contact (A) with the hole created by the previous drilling and the secondary contact (B) with the sleeve.
 - > Create the hole using the initial drill and insert the next drill into the hole made during the previous step and drill after achieving the drill and sleeve contact (A&B).
 - > If drilling only with the sleeve contact (B) without the drill contact (A), the path may not be correct.




* Precaution when irrigating

- > Irrigate enough to the end of the drill hole.



Drilling Sequence

> Total drilling sequence with the Tissue Punches, Bone Flattening Drills, Initial Drills, and Pilot Drills, Abutment Profilers, and Implant Adapters.



InnoFit Lodestar Kit [KLS001]

- > A cost-effective guided surgery solution applicable to various types of clinical cases.
- > Universal to any implant system.




Pilot Drill(Ø2.0)

KLSPD2007 KLSPD2008 KLSPD2010 KLSPD2012 KLSPD2014



Pilot Drill(Ø2.7)

KLSPD2707 KLSPD2708 KLSPD2710 KLSPD2712 KLSPD2714




Pilot Drill(Ø3.4)

KLSPD3407 KLSPD3408 KLSPD3410 KLSPD3412 KLSPD3414



Pilot Drill(Ø4.2)


KLSPD4207 KLSPD4208 KLSPD4210 KLSPD4212 KLSPD4214



Tissue Punch
KLSTP45



Initial Drill
KLSID18 KLSID18L

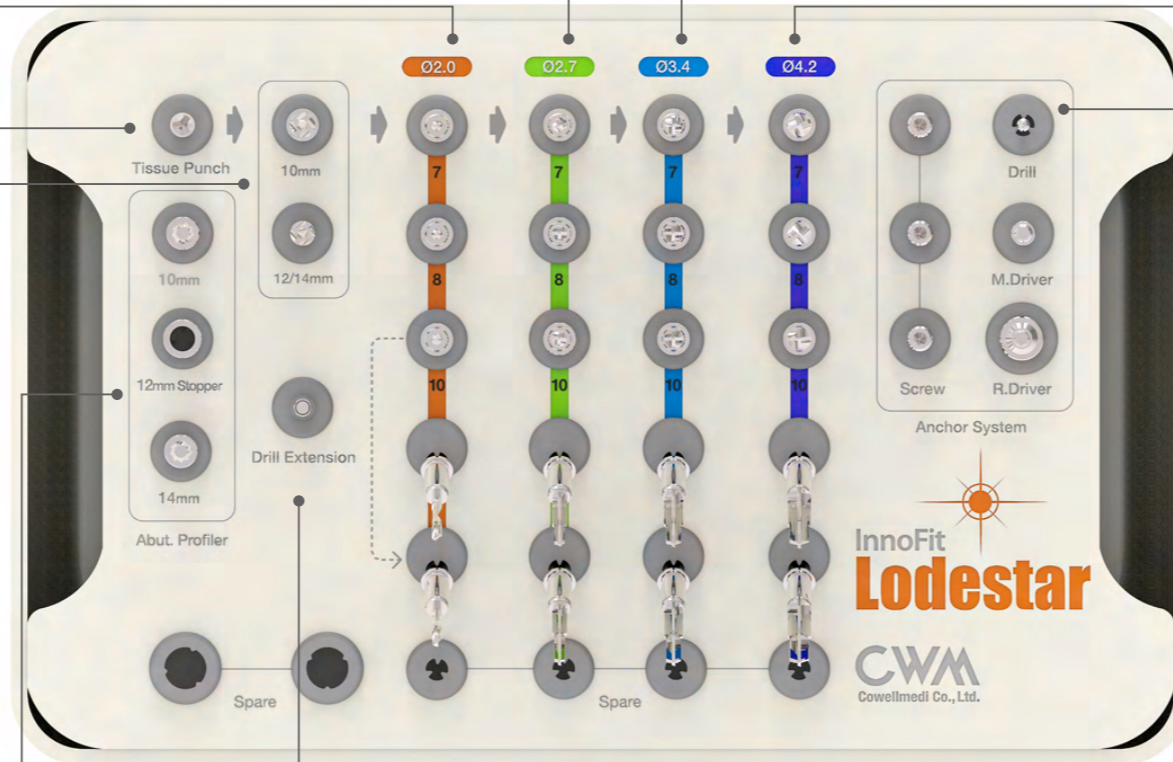

Abut. Profiler
KLSPD10 KLSPD12S KLSPD14




Drill Extension
KDE002




Anchor System
KLSAD13 KLSAS18 KLSMD23 KLSRD16

Tissue Punch


> The gingiva in the position where the implant is to be placed can be incised in a circular shape and can also be used in inclined bones (50rpm without irrigation).



KLSTP45



The gingiva can be incised in a circular shape although the bone level is inclined or not parallel.




The internal cutting edge of the Tissue Punch cuts the gingiva into small pieces so that those can be removed by suction without extra work.




Initial Drill


> The Drill combined with Bone Flattening Drill and Point Drill which no separate Bone Flattening Drill is required provides a simpler procedure and shorter chair time (1,000rpm with irrigation).



KLSID18



KLSID18L



Point


Bone Flattening
Flattens uneven surface of the alveolar crest.

Creates the hole on the bone surface so that the axis of the next step Drill is not moved and it guides the Drill position by preventing slip even at the inclined bone level.

Pilot Drill


> Ø2.0 / Ø2.7 / Ø3.4 / Ø4.2.

Ø2.0: High Speed - 600rpm




Pilot Drill 16mm(6mm)

KLSPD2007




Pilot Drill 17mm(7mm)

KLSPD2008




Pilot Drill 19mm(9mm)

KLSPD2010



Pilot Drill 21mm(11mm)


KLSPD2012



Pilot Drill 23mm(13mm)

KLSPD2014

Ø2.7 / Ø3.4 / Ø4.2: Low Speed - 50~200rpm / 50N.cm




Pilot Drill 17mm(7mm)

KLSPD2707

KLSPD3407

KLSPD4207




Pilot Drill 19mm(9mm)

KLSPD2708

KLSPD3408

KLSPD4208




Pilot Drill 21mm(11mm)

KLSPD2710

KLSPD3410

KLSPD4210




Pilot Drill 23mm(13mm)

KLSPD2712

KLSPD3412

KLSPD4212



Pilot Drill 25mm(15mm)


KLSPD2714

KLSPD3414

KLSPD4214


Abutment Profiler

> Used for the elimination of the alveolar bone that interferes with the accurate connection of abutment.




* Comprehension and Usage of Offset

- > The basic length from the fixture platform to the top of the Sleeve is 10mm.
- > In case the gingival is thick or fixture needs to be placed deeper due to low bone density, use the Sleeve 2 or 4mm upright to the top.
- > The higher the offset value, the less accurate it is, so use 10mm if possible.



Anchor System



* Packing Unit: 5 Sleeves

Optional


> These products are optional as extra ones which are not included in the kit.

Guide Reamer *Extra*



Used for precise contact of Drill and Sleeve (Sleeve / Non-Sleeve).

Use the 4.5mm Guide Reamer for Non-Sleeve, and the 5.3 Guide Reamer for Sleeve (800rpm without irrigation).

Guide Reamer (Non-Sleeve)
KLSRD45




Guide Reamer (Sleeve)
KLSRD53



Non Sleeve
KLSRD45


Revises imprecisely formed hole after the guided template fabrication using the 4.5 Guide Reamer to create the hole to be in exact contact with the Drill.



Sleeve
KLSRD53


Revises imprecisely formed hole after the guided template fabrication using the 5.3mm Guide Reamer to precisely insert the Sleeve.

Sleeve *Extra*




Closed Sleeve
KLSS01

* Packing Unit: 5 Sleeves




Open Sleeve
KLSS02


* Packing Unit: 5 Sleeves




Pilot Drill – 16/18mm *Extra*




KLSPD2018



KLSPD2718




KLSPD3418




Drilling Sequence

Drilling Sequence (Non Sleeve)




Drilling Sequence (Sleeve)



* Use 10mm Drill prior to 14mm Drill


For the use of the 14mm Drill with accurate contact to the Sleeve, use the Ø2.0x10mm Drill before using the 14mm Drill.

e.g.) 3.4 X 14mm Drilling Sequence




* Drilling method

- > Make sure with drilling in the desired direction without a change in the path through the primary Drill contact (A) with the hole created by the previous drilling and the secondary contact (B) with the Sleeve.
- > Create the hole using the Initial Drill and insert the next drill into the hole made during the previous step and Drill after achieving the Drill and Sleeve contact (A&B).
- > If drilling only with the Sleeve contact (B) without the Drill contact (A), the path may not be correct.




* Precaution when irrigating

- > Irrigate enough to the end of the drill hole.




Drilling Sequence

> Total drilling sequence with the Tissue Punches, Initial Drills, Pilot Drills, and Abutment Profilers.




Component selection guide for the Sub. Hybrid Ti-Base System

- Intra-oral scanning
- Model-scanning

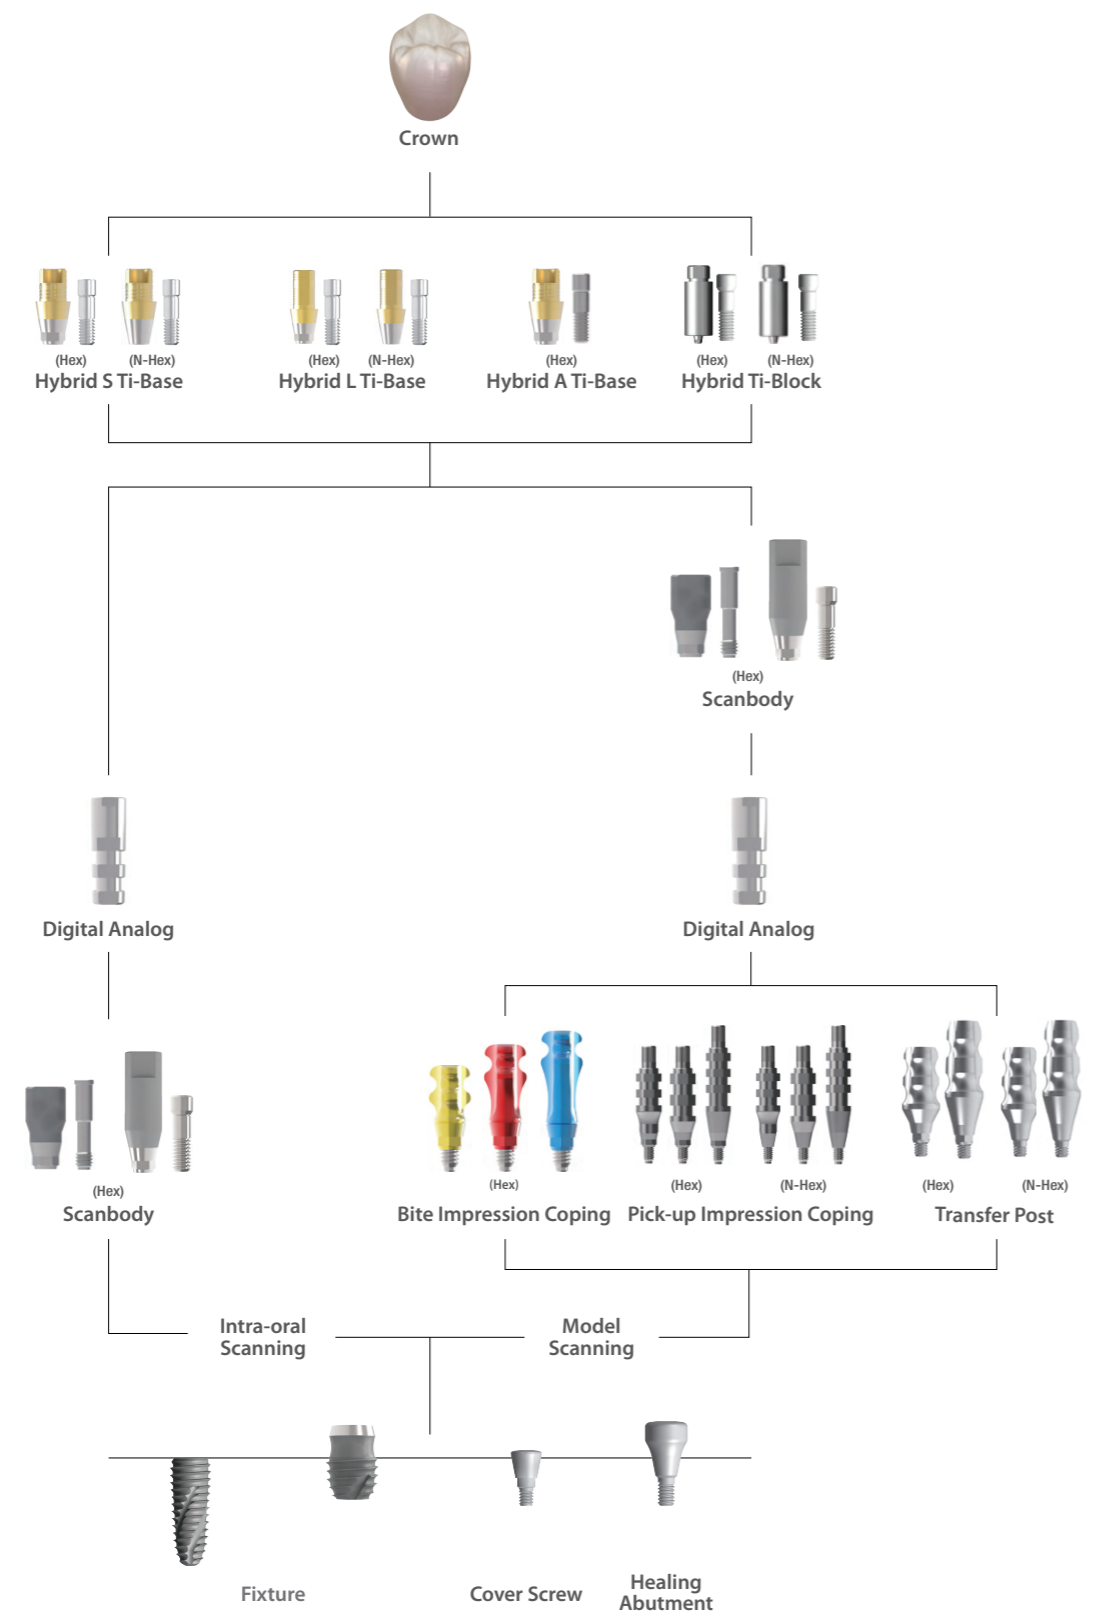


Hybrid S Ti-Base



Type	Hex			N-Hex
Diameter	Ø4.0	Ø5.0	Ø6.0	Ø4.0
Length	3.75	3.75	3.75	3.75
0.8	2SLH404	2SLH504	2SLH604	2SLN404
2	2SLH424	2SLH524	2SLH624	2SLN424
3	2SLH434	2SLH534	2SLH634	2SLN434

- > Packing unit: 1 Hybrid S Ti-Base + 1 Abutment Screw.
- > For Screw-Cement or Cement Retained Abutment.
- > Titanium base for the strength of CAD/CAM customized abutment or crown.
- > Gold color for more translucent restoration.
- > Lingual surface hole for more esthetic restoration (Ø4.0).
- > Right angled (Ø4.0) and humped design (Ø5.0, Ø6.0) for anti-rotation of the prosthesis.
- > Library available for EXOCAD®, 3Shape® & Others.
- > Connected with the Abutment Screw (2SSHR200).
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 30N.cm.
- > Use the Scanbody for 3D Work.
- > Fixture level impression.


Hybrid L Ti-Base



Type	Hex			N-Hex
Diameter	Ø4.0	Ø5.0	Ø6.0	Ø4.0
Length	5.5	5.5	5.5	5.5
1	2SLH415	2SLH515	2SLH615	2SLN415
2	2SLH425	2SLH525	2SLH625	2SLN425
3	2SLH435	2SLH535	2SLH635	2SLN435

- > Packing unit: 1 Hybrid L Ti-Base + 1 Abutment Screw.
- > For Screw-Cement or Cement Retained Abutment.
- > Titanium base for the strength of CAD/CAM customized abutment or crown.
- > Gold color for more translucent restoration.
- > Cutting surface (Ø4.0) and humped design (Ø5.0, Ø6.0) for anti-rotation of the prosthesis.
- > Library available for EXOCAD®, 3Shape® & Others.
- > Connected with the Abutment Screw (2SSHR200).
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 30N.cm.
- > Use the Scanbody for 3D Work.
- > Fixture level impression.

Hybrid A Ti-Base



Type	Hex	N-Hex
Diameter	Ø4.0	Ø4.0
Length / Cuff	3.75	3.75
0.8	2SLH404A	2SLN404A
2	2SLH424A	2SLN424A
3	2SLH434A	2SLN434A

- > Packing unit: 1 Hybrid A Ti-Base + 1 Abutment Screw.
- > For Screw-Cement or Cement Retained Abutment.
- > Titanium base for the strength of CAD/CAM customized abutment or crown.
- > For Fabrication of Angulated Screw Channel up to 25°.
- > Library available for EXOCAD®, 3Shape® & Others.
- > Connected with the Stargrip Abutment Screw (2SLAH100, 2SLAH200 & 2SLAH300).
- > Tightened with the Angulated Screw Ratchet Driver and Torque Wrench.
- > Tightening torque force: 30N.cm.
- > Use the Scanbody for 3D Work.
- > Fixture level impression.

* Angulated Screw Ratchet Driver

Height / Type	Ratchet
24(Short)	KRBUD15
29(Long)	KRBUD20

- > Stable to internal slip or fracture due to wide contact area of the Angulated Driver and the dedicated Stargrip Abutment Screw.
- > Tightening torque force: 30N.cm (50N.cm Max.).


Bite Impression Coping



Type	Hex(Short)	Hex(Long)	Hex(X-Long)
Diameter	Ø4.5	Ø4.5	Ø4.5
Length / Cuff	2	4	6
4.0	2SBIC45S	2SBIC45L	2SBIC45X

- > Packing unit: 1 Bite Impression Coping (Inbuilt Guide Pin).
- > Designed to simultaneously take bite and impression.
- > For closed tray impression (Bite Impression).
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 12~15N.cm.


Hybrid Ti-Block



Type	Hex			N-Hex		
Diameter / Length	10	12	14	10	12	14
20	CSHH10S	CSHH12S	CSHH14S	CSHN10S	CSHN12S	CSHN14S

- > Packing unit: 1 Hybrid Ti-Block + 2 Abutment Screws.
- > For Screw-Cement or Cement Retained Abutment.
- > Block abutment for CAD/CAM customized abutment.
- > Library available for EXOCAD®, 3Shape® & Others.
- > Connected with the Abutment Screw (2SSH100).
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 30N.cm.
- > Use the Scanbody for 3D Work.
- > Fixture level impression.


Pick-up Impression Coping



Type	Hex			N-Hex		
Diameter / Length / Cuff	Ø4.5	Ø5.5	Ø6.5	Ø4.5	Ø5.5	Ø6.5
12 (Short) / 4	2SIH454S	2SIH554S	2SIH654S	2SIN454S	2SIN554S	2SIN654S
14 (Short) / 2	2SIH45S	2SIH55S	2SIH65S	2SIN45S	2SIN55S	2SIN65S
16 (Long) / 4	2SIH45L	2SIH55L	2SIH65L	2SIN45L	2SIN55L	2SIN65L

- > Packing unit: 1 Pick-up Impression Coping + 1 Guide Pin.
- > For open tray impression.
- > Connected with the Guide Pin (2SISR001SS / 2SISR001SL).
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 12~15N.cm.


Scanbody



Type	Hex(Short)	Hex(Long)
Diameter	Ø4.3	Ø4.3
Height	6	11
Length / Cuff	4	9
2	2SSB4325	2SSB4329

- > Packing unit: 1 Scanbody + 1 Abutment Screw.
- > For both, model-scanner and intra-oral scanner.
- > Made of 100% titanium alloy with a special coating applied.
- > No need to spray.
- > Connected with the Abutment Screw.
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 12~15N.cm.


Transfer Post



Type	Hex			N-Hex		
Diameter / Length / Cuff	Ø4.5	Ø5.5	Ø6.5	Ø4.5	Ø5.5	Ø6.5
9 (Short) / 2	2STH45S	2STH55S	2STH65S	2STN45S	2STN55S	2STN65S
11 (Long) / 4	2STH45L	2STH55L	2STH65L	2STN45L	2STN55L	2STN65L

- > Packing unit: Hex - 1 Transfer Post + 1 Guide Pin / N-Hex - 1 Transfer Post (Solid Type).
- > For closed tray impression.
- > Connected with the Guide Pin (2STH001SS / 2STH001SL).
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 12~15N.cm.

Abutment Screw



Diameter / Height	Ø2.45	Ø2.15	Ø2.15
8.5	2SSHR100	2SSHR200	
10.7			2SSHR100S

- > Packing unit: 1 Abutment Screw.
- > 2SSHR100: Hybrid Block and Scanbody (2SSB4329).
- > 2SSHR200: Hybrid S Ti-Base and Hybrid L Ti-Base.
- > 2SSHR100S: Scanbody (2SSB4325).
- > Tightened with the 1.2 Hex Driver and Torque Wrench.


Digital Analog



Diameter / Height	Ø3.9
12	2SDR001

- > Packing unit: 1 Digital Analog.
- > Analog of fixture for the working cast.
- > Used for both 3D printed model (RP) and stone model.

A Abutment Screw




Diameter / Height	2	3.2	4.2
Ø2.15	2SLAH100	2SLAH200	2SLAH300


- > Packing unit: 1 A Abutment Screw.
- > Exclusive for the Hybrid A Ti-Base (2SLAH100 for 2SLH404A, 2SLAH200 for 2SLH424A & 2SLAH300 for 2SLH434A).
- > Tightened with the Angulated Screw Driver and Torque Wrench.

Component selection guide for the Sub. & Sub-N. Multi Hybrid Ti-Base System

- Intra-oral scanning
- Model-scanning

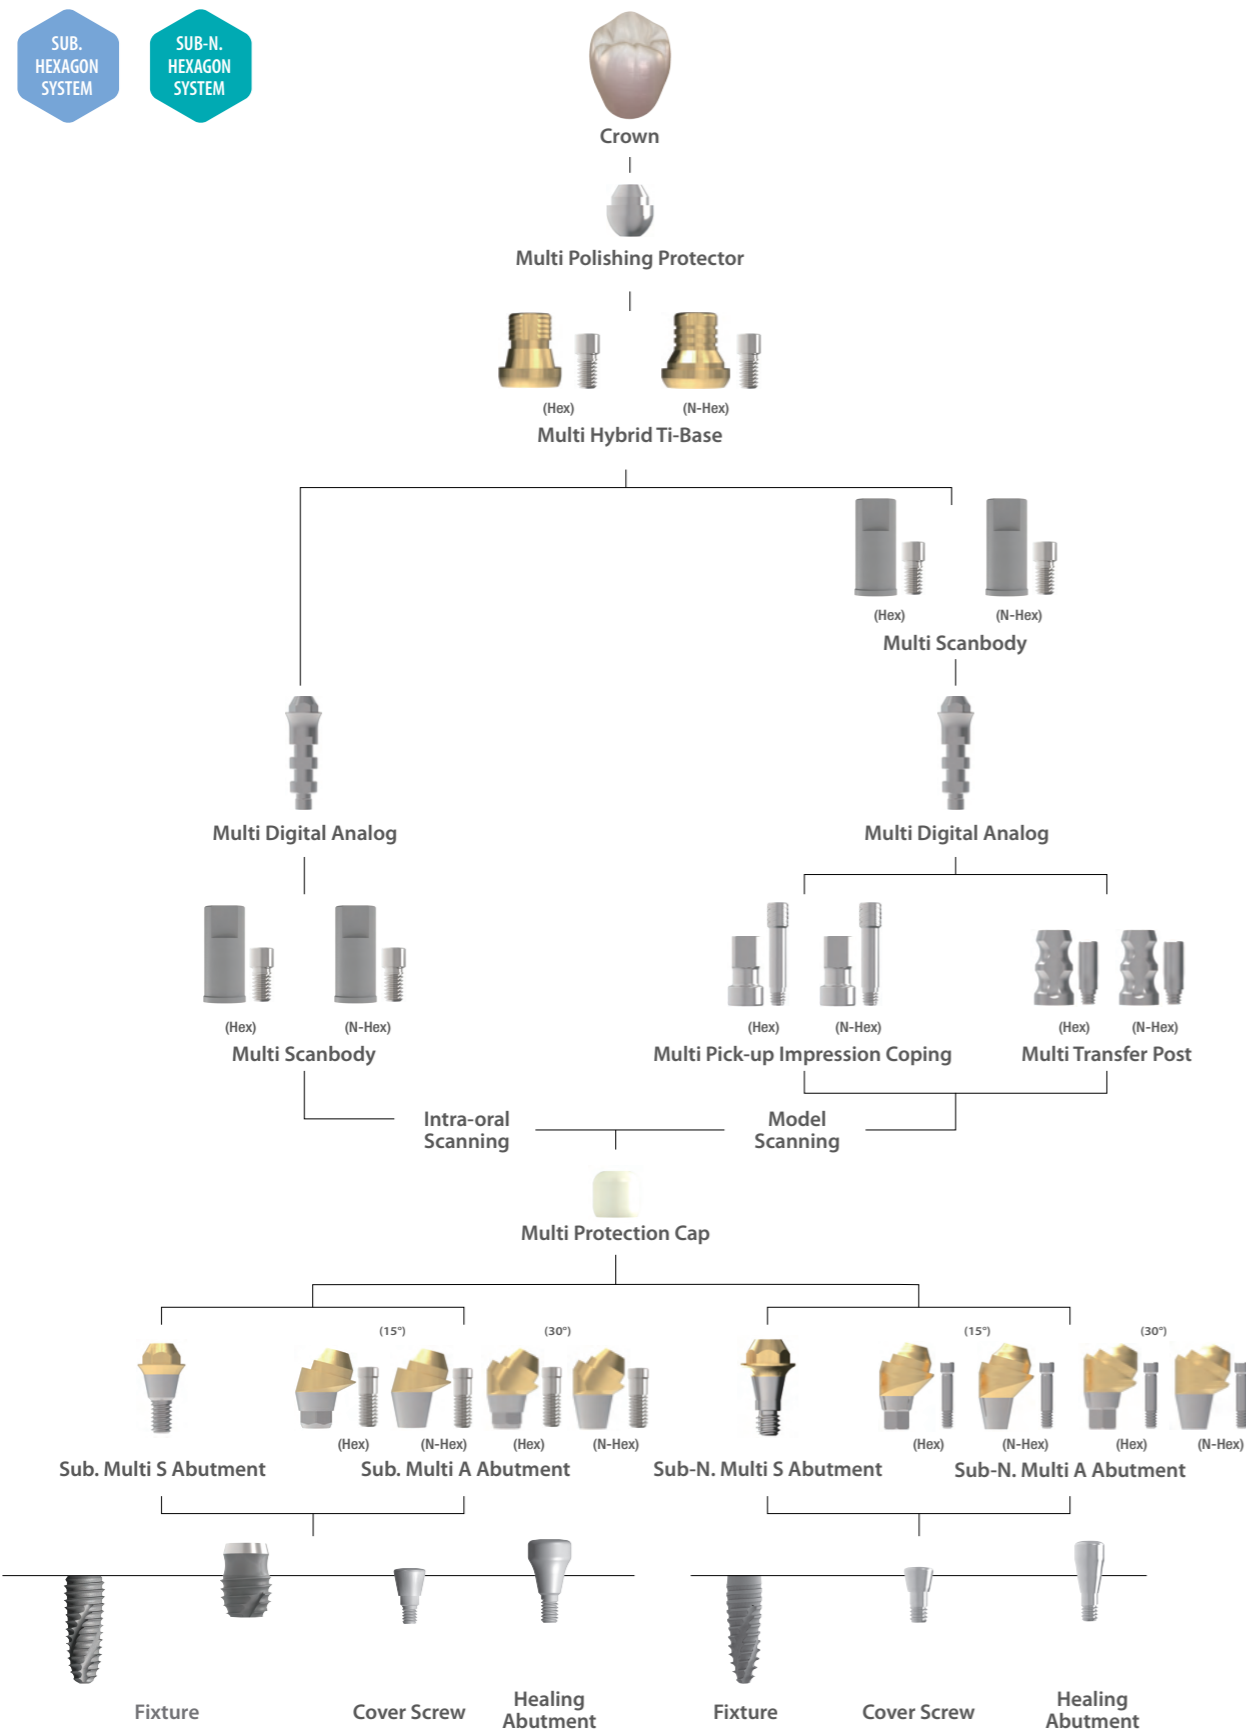


Multi S Abutment



Fixture Connection	Hex2.1[Sub-N.]	Hex2.5[Sub.]	
Platform[Fixture Dia.]	Ø4.5 [Ø3.1 / Ø3.3]	Ø4.5 [Ø3.5 / Ø4.0 / Ø4.5 / Ø5.0 / Ø6.0]	
Diameter	Ø4.5	Ø4.5	Ø5.5
Cuff Length	2	2	2
1	SMS451N	2SMS451	2SMS551
2	SMS452N	2SMS452	2SMS552
3	SMS453N	2SMS453	2SMS553
4	SMS454N	2SMS454	2SMS554
5		2SMS455	2SMS555

- > Packing unit: 1 Multi S Abutment.
- > For Screw-Retained Prosthesis.
- > Titanium base for the Multi Hybrid Ti-Base.
- > Gold color for more translucent restoration.
- > Library available for EXOCAD®, 3Shape® & others.
- > Integrated with the screw and abutment (solid screw).
- > Use the S Holder for a more stable position.
- > Tightened with the S Machine or S Ratchet Driver and Torque Wrench.
- > Tightening torque force: 30N.cm (Sub.) / 20~25N.cm (Sub-N).
- > Use the Multi Scanbody for digital flow.
- > Abutment level impression.

Multi A Abutment




Type	Hex					
Fixture Connection	Hex2.1[Sub-N.]		Hex2.5[Sub.]			
Platform[Fixture Dia.]	Ø4.5 [Ø3.1 / Ø3.3]		Ø4.5 [Ø3.5 / Ø4.0 / Ø4.5 / Ø5.0 / Ø6.0]		Ø5.5 [Ø3.5 / Ø4.0 / Ø4.5 / Ø5.0 / Ø6.0]	
Diameter(Angle)	Ø4.5(15°)	Ø4.5(30°)	Ø4.5(15°)	Ø4.5(30°)	Ø5.5(15°)	Ø5.5(30°)
Cuff Length	2	2	2	2	2	2
2	★ SMAH45152N		★ ZSMAH45152			
3	★ SMAH45153N	★ SMAH45303N	★ ZSMAH45153	★ ZSMAH45303	★ ZSMAH55153	★ ZSMAH55303
4	★ SMAH45154N	★ SMAH45304N	★ ZSMAH45154	★ ZSMAH45304	★ ZSMAH55154	★ ZSMAH55304
5					★ ZSMAH55155	★ ZSMAH55305

Type	N-Hex					
Fixture Connection	Hex2.1[Sub-N.]		Hex2.5[Sub.]			
Platform[Fixture Dia.]	Ø4.5 [Ø3.1 / Ø3.3]		Ø4.5 [Ø3.5 / Ø4.0 / Ø4.5 / Ø5.0 / Ø6.0]		Ø5.5 [Ø3.5 / Ø4.0 / Ø4.5 / Ø5.0 / Ø6.0]	
Diameter(Angle)	Ø4.5(15°)	Ø4.5(30°)	Ø4.5(15°)	Ø4.5(30°)	Ø5.5(15°)	Ø5.5(30°)
Cuff Length	2	2	2	2	2	2
2	★ SMAN45152N		★ ZSMAN45152			
3	★ SMAN45153N	★ SMAN45303N	★ ZSMAN45153	★ ZSMAN45303	★ ZSMAN55153	★ ZSMAN55303
4	★ SMAN45154N	★ SMAN45304N	★ ZSMAN45154	★ ZSMAN45304	★ ZSMAN55154	★ ZSMAN55304
5					★ ZSMAN55155	★ ZSMAN55305

- > Packing unit: 1 Multi A Abutment + 1 Abutment Screw.
- > For Screw-Retained Prosthesis.
- > Titanium base for the Multi Hybrid Ti-Base.
- > Gold color for more translucent restoration.
- > Library available for EXOCAD®, 3Shape® & others.
- > Use the A Holder for a more stable position.
- > Connected with the Abutment Screw (SSHR200N: ★ SSSHR300N: ● / 2SSHR300: ★ 2SSHR400: ●).
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 30N.cm (Sub.) / 20~25N.cm (Sub-N).
- > Use the Multi Scanbody for digital flow.
- > Abutment level impression.


Abutment Screw



Height	8.7	9.3	7.5	6.5
Diameter	★ SSHR200N	● SSHR300N		
			★ 2SSHR300	● 2SSHR400

- > Packing unit: 1 Abutment Screw.
- > To connect the Multi A Abutment.
- > Tightened with the 1.2 Hex Driver and Torque Wrench.


Multi Protection Cap



Multi S & A Abutment Diameter	Ø4.5	Ø5.5
Diameter	Ø5.2	Ø6.2
Height	5	5

- > Packing unit: 1 Multi Protection Cap.
- > Protection from cheek and tongue for gingival healing period.
- > Gingival retraction for prosthodontic margin of the abutment.
- > Alternative usage for sub-structure of the temporary prosthesis.
- > Tightened with the 1.2 Hex Driver.
- > Tightening torque force: 5~10N.cm.


Multi Scanbody



Type	Hex	N-Hex
Multi S & A Abutment Diameter	Ø4.5 & Ø5.5	Ø4.5 & Ø5.5
Diameter	Ø4.5	Ø4.5
Height	9	9

- > Packing unit: 1 Multi Scanbody + 1 Multi Cylinder Screw.
- > For both, model-scanner and intra-oral scanner.
- > For the Multi Hybrid Ti-Base.
- > Made of 100% titanium alloy with a special coating applied.
- > No need to spray.
- > Connected with the Multi Cylinder Screw (2SMCS100).
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 12~15N.cm.


Multi Pick-up Impression Coping



Type	Hex	N-Hex
Multi S & A Abutment Diameter	Ø4.5	Ø5.5
Diameter	Ø4.65	Ø5.65
Height	14.8	14.8

- > Packing unit: 1 Multi Pick-up Impression Coping + 1 Guide Pin.
- > For open tray impression.
- > Connected with the Guide Pin (2SMGP012).
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 12~15N.cm.

Multi Transfer Post



Type	Hex		N-Hex	
Multi S & A Abutment Diameter	Ø4.5	Ø5.5	Ø4.5	Ø5.5
Diameter	Ø4.5	Ø5.5	Ø4.5	Ø5.5
Height	8.5	8.5	8.5	8.5

- > Packing unit: 1 Multi Transfer Post + 1 Guide Pin.
- > For closed tray impression.
- > Connected with the Guide Pin (2SMTHS100).
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 12~15N.cm.


Multi Digital Analog



Multi S & A Abutment Diameter	Ø4.5	Ø5.5
Diameter	Ø4.5	Ø5.5
Length	2	2

- > Packing unit: 1 Multi Digital Analog.
- > Replacement of the Multi S or A Abutment shape in working cast.
- > Used for both 3D printed model (RP) and stone model.
- > Select according to the dimension of the Multi S or A Abutment.


Multi Hybrid Ti-Base



Type	Hex			N-Hex		
Multi S & A Abutment Diameter	Ø4.5	Ø4.5	Ø5.5	Ø4.5	Ø4.5	Ø5.5
Diameter	Ø4.5	Ø4.5	Ø5.5	Ø4.5	Ø4.5	Ø5.5
Length	4.5	4.5	4.5	4.5	4.5	4.5
Cuff	0.5	0.5	0.5	0.5	0.5	0.5

- > Packing unit: 1 Multi Hybrid Ti-Base + 1 Multi Cylinder Screw.
- > For Screw-Cement or Cement Retained Abutment.
- > Titanium base for the strength of CAD/CAM customized abutment or crown.
- > Gold color for more translucent restoration.
- > Cutting surface for anti-rotation of the prosthesis.
- > Library available for EXOCAD®, 3Shape® & Others.
- > Connected with the Multi Cylinder Screw (2SMCS100).
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 20N.cm.
- > Use the Scanbody for 3D Work.
- > Abutment level impression.

Multi Cylinder Screw




Diameter	Ø2.25
Height	5

- > Packing unit: 1 Multi Cylinder Screw.
- > Connected with the Multi Scanbody and Multi Hybrid Ti-Base.
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 20N.cm.


Component selection guide for the Sub. Lock Hybrid Ti-Base System



- Intra-oral scanning
- Model-scanning

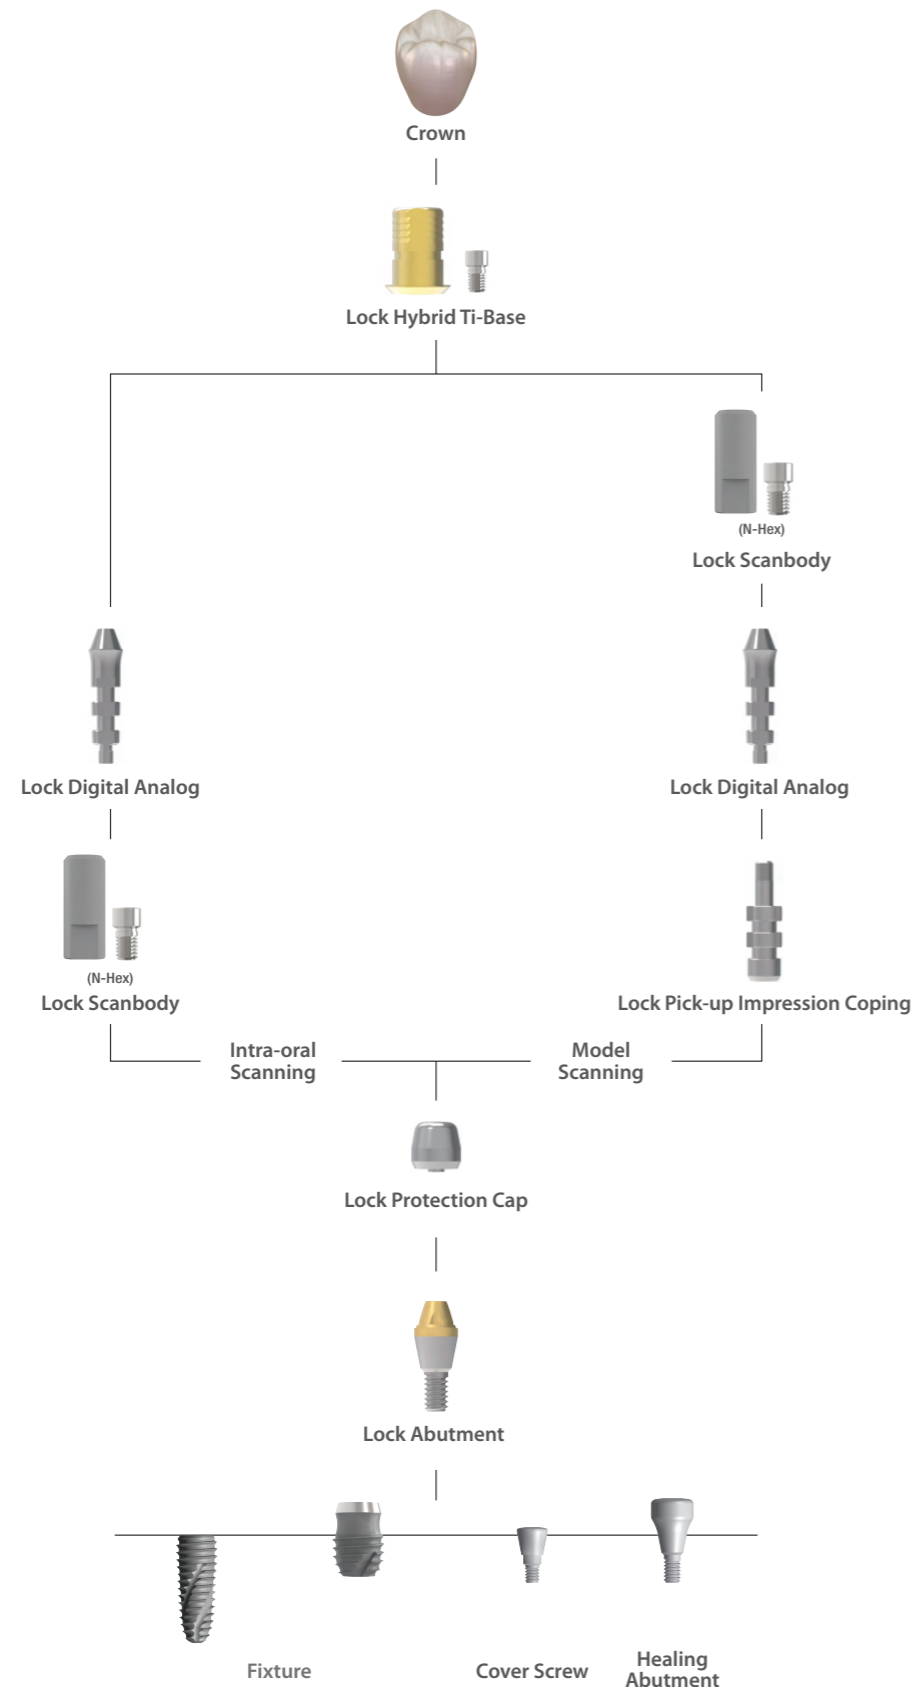


Lock Abutment



Diameter	Ø3.5
Cuff Length	2.15
0.5	2SLA400
1	2SLA410
2	2SLA420
3	2SLA430
4	2SLA440

- > Packing unit: 1 Lock Abutment.
- > For Screw-Retained Prosthesis.
- > Titanium base for the Lock Hybrid Ti-Base.
- > Gold color for more translucent restoration.
- > Integrated with screw and abutment.
- > Tightened with the Lock Ratchet Driver and Torque Wrench.
- > Tightening torque force: 30N.cm.
- > Abutment level impression.


Lock Protection Cap



Lock Abutment Diameter	Ø3.5
Diameter	Ø4.3
Height	4
	2SLP45

- > Packing unit: 1 Lock Protection Cap.
- > Protection from cheek and tongue for gingival healing period.
- > Gingival retraction for prosthodontic margin of the abutment.
- > Tightened with the 1.2 Hex Driver.
- > Tightening torque force: 5~10N.cm.


Lock Scanbody



Lock Abutment Diameter	Ø3.5
Diameter	Ø4.3
Height	9
	2SLB001H

- > Packing unit: 1 Lock Scanbody + 1 Lock Cylinder Screw.
- > For both, model scanner and intra oral scanner.
- > For the Lock Hybrid Ti-Base.
- > Made of 100% titanium alloy with a special coating applied.
- > No need to spray.
- > Connected with the Lock Cylinder Screw (2SLCS200).
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 12~15N.cm.

Lock Pick-up Impression Coping



Lock Abutment Diameter	Ø3.5
Diameter	Ø4.3
Height	16
	2SLIH45

- > Packing unit: 1 Lock Pick-up Impression Coping + 1 Guide Pin.
- > Connected with the Guide Pin (2SLIH45S).
- > For open tray impression.


Lock Digital Analog



Lock Abutment Diameter	Ø3.5
Diameter	Ø3.5
Length	2.2
	2SLLA35

- > Packing unit: 1 Lock Digital Analog.
- > Used for both 3D printed model (RP) and stone model.


Lock Hybrid Ti-Base



Lock Abutment Diameter	Ø3.5
Diameter	Ø4.5
Length	5
Cuff	0.5
	2SLHT40N

- > Packing unit: 1 Lock Hybrid Ti-Base + 1 Lock Cylinder Screw.
- > For Screw-Cement or Cement Retained Abutment.
- > Titanium base for the strength of CAD/CAM customized abutment or crown.
- > Gold color for more translucent restoration.
- > Cutting surface for anti-rotation of the prosthesis.
- > Library available for EXOCAD®, 3Shape® & Others.
- > Connected with the Lock Cylinder Screw (2SLCS200).
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 30N.cm.
- > Use the Scanbody for 3D Work.
- > Abutment level impression.



Lock Cylinder Screw



Diameter	Ø2.3
Height	4.8
	2SLCS200


- > Packing unit: 1 Lock Cylinder Screw.
- > Connected with the Lock Scanbody and Lock Hybrid Ti-Base.
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 30N.cm.

Lock Ratchet Driver



Type	Ratchet
Height	14.2
	KRLRD18
	28.5
	KRLRD28


- > Packing unit: 1 Lock Ratchet Driver.
- > To install and remove the Lock Abutment with the Torque Wrench.




Component selection guide for the Sub-N. Hybrid Ti-Base System



- Intra-oral scanning
- Model-scanning

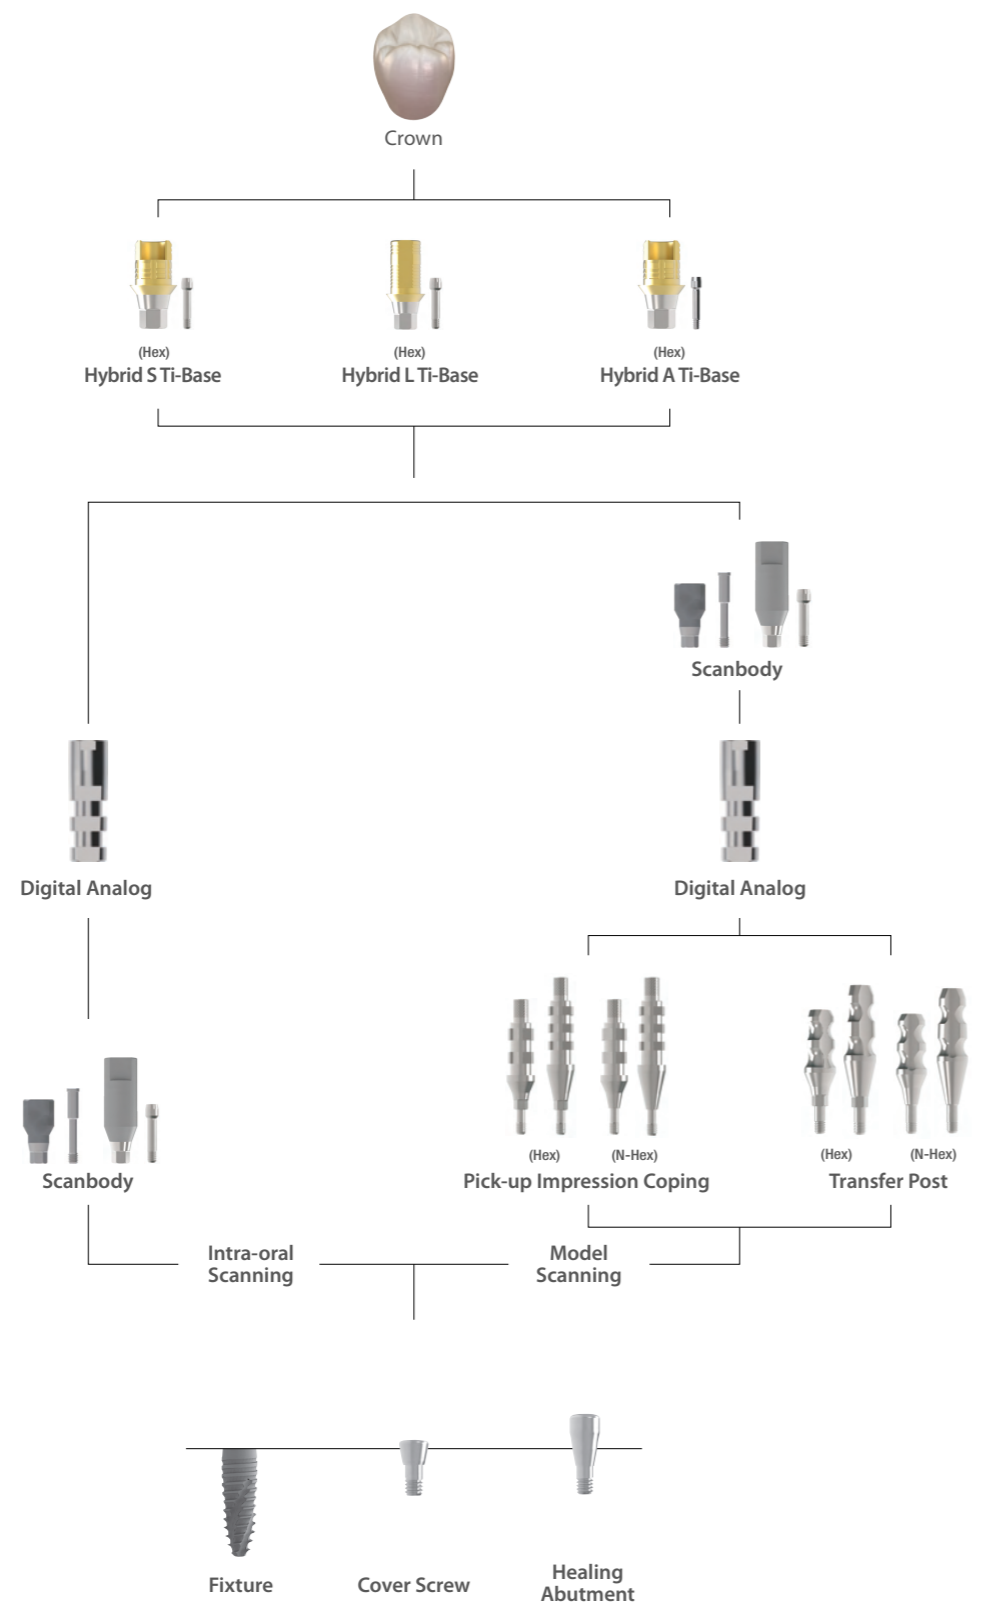


Hybrid S Ti-Base



Type	Hex
Diameter	Ø4.0
Length Cuff	3.75
0.8	SLH404N
2	SLH424N
3	SLH434N

- > Packing unit: 1 Hybrid S Ti-Base + 1 Abutment Screw.
- > For Screw-Cement or Cement Retained Abutment.
- > Titanium base for the strength of CAD/CAM customized abutment or crown.
- > Gold color for more translucent restoration.
- > Lingual surface hole for more esthetic restoration.
- > Right angled for anti-rotation of the prosthesis.
- > Library available for EXOCAD®, 3Shape® & Others.
- > Connected with the Abutment Screw (SSHR100N).
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 20~25N.cm.
- > Use the Scanbody for 3D Work.
- > Fixture level impression.


Hybrid L Ti-Base



Type	Hex
Diameter	Ø4.0
Length Cuff	5.5
1	SLH415N
2	SLH425N
3	SLH435N

- > Packing unit: 1 Hybrid L Ti-Base + 1 Abutment Screw.
- > For Screw-Cement or Cement Retained Abutment.
- > Titanium base for the strength of CAD/CAM customized abutment or crown.
- > Gold color for more translucent restoration.
- > Cutting surface for anti-rotation of the prosthesis.
- > Library available for EXOCAD®, 3Shape® & Others.
- > Connected with the Abutment Screw (SSHR100N).
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 20~25N.cm.
- > Use the Scanbody for 3D Work.
- > Fixture level impression.

Hybrid A Ti-Base



Type	Hex	N-Hex
Diameter	Ø4.0	Ø4.0
Length Cuff	3.75	3.75
0.8	2SLH404AN	2SLN404AN
2	2SLH424AN	2SLN424AN
3	2SLH434AN	2SLN434AN


- > Packing unit: 1 Hybrid A Ti-Base + 1 Abutment Screw.
- > For Screw-Cement or Cement Retained Abutment.
- > Titanium base for the strength of CAD/CAM customized abutment or crown.
- > For Fabrication of Angulated Screw Channel up to 25°.
- > Right angled for anti-rotation of the prosthesis.
- > Library available for EXOCAD®, 3Shape® & Others.
- > Connected with the Stargrip Abutment Screw (SLAH100N, SLAH200N & SLAH300N).
- > Tightened with the Angulated Screw Ratchet Driver and Torque Wrench.
- > Tightening torque force: 20~25N.cm.
- > Use the Scanbody for 3D Work.
- > Fixture level impression.

* Angulated Screw Ratchet Driver

Height	Type	Ratchet
24(Short)		KRBUD15
29(Long)		KRBUD20

- > Stable to internal slip or fracture due to wide contact area of the Angulated Driver and the dedicated Stargrip Abutment Screw.
- > Tightening torque force: 30N.cm (50N.cm Max.).

Scanbody



Type	Hex(Short)	Hex(Long)
Diameter	Ø4.3	Ø4.3
Height	6	11
Length / Cuff	4	9
2	SSB4325N	SSB4329N

- > Packing unit: 1 Scanbody + 1 Abutment Screw.
- > For both, model-scanner and intra-oral scanner.
- > Made of 100% titanium alloy with a special coating applied.
- > No need to spray.
- > Connected with the Abutment Screw.
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 12~15N.cm.


Digital Analog



Diameter	Ø3.9
Height	SDR001N
12	

- > Packing unit: 1 Digital Analog.
- > Analog of fixture for the working cast.
- > Used for both 3D printed model (RP) and stone model.


Pick-up Impression Coping



Type	Hex	N-Hex
Diameter	Ø4.5	Ø4.5
Length / Cuff		
14 (Short) / 2	SIH45SN	SIN45SN
16 (Long) / 4	SIH45LN	SIN45LN

- > Packing unit: 1 Pick-up Impression Coping + 1 Guide Pin.
- > For open tray impression.
- > Connected with the Guide Pin (SIS001SN / SIS001LN).
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 12~15N.cm.


Abutment Screw



Diameter	Ø2.25	Ø1.95
Height	SSH100N	SSB100SN
10.2		
12.3		

- > Packing unit: 1 Abutment Screw.
- > SSH100N: Hybrid S Ti-Base, Hybrid L Ti-Base, and Scanbody (SSB4329N).
- > SSB100SN: Scanbody (SSB4325N).
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 20~25N.cm.


Transfer Post



Type	Hex	N-Hex
Diameter	Ø4.5	Ø4.5
Length / Cuff		
9 (Short) / 2	STH45SN	STN45SN
11 (Long) / 4	STH45LN	STN45LN

- > Packing unit: Hex - 1 Transfer Post + 1 Guide Pin / N-Hex - 1 Transfer Post (Solid Type).
- > For closed tray impression.
- > Connected with the Guide Pin (STS001SN / STS001LN).
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 12~15N.cm.

A Abutment Screw




Height	10.2	11.4	12.4
Diameter	SLAH100N	SLAH200N	SLAH300N
Ø2.25			


- > Packing unit: 1 A Abutment Screw.
- > Exclusive for the Hybrid A Ti-Base (SLAH100N for SLH404AN, SLAH200N for SLH424AN & SLAH300N for SLH434AN).
- > Tightened with the Angulated Screw Driver and Torque Wrench.

Component selection guide for the Int. Hybrid Ti-Base System

- Intra-oral scanning
- Model-scanning




Hybrid S Ti-Base



Type	Octa		N-Octa	
Platform [Fixture Dia.]	Ø4.8 [Ø3.5 / Ø4.0 / Ø4.5]	Ø5.9 [Ø5.0 / Ø6.0]	Ø4.8 [Ø3.5 / Ø4.0 / Ø4.5]	Ø5.9 [Ø5.0 / Ø6.0]
Diameter	Ø5.1	Ø6.2	Ø5.1	Ø6.2
Length	4	4	4	4
Cuff				
0.8	ILO4814	ILO5914	ILN4814	ILN5914
2	ILO4824	ILO5924	ILN4824	ILN5924
3	ILO4834	ILO5934	ILN4834	ILN5934

- > Packing unit: 1 Hybrid S Ti-Base + 1 Abutment Screw.
- > For Screw-Cement or Cement Retained Abutment.
- > Titanium base for the strength of CAD/CAM customized abutment or crown.
- > Gold color for more translucent restoration.
- > Library available for EXOCAD®, 3Shape® & others.
- > Right angled (Ø5.1) and humped design (Ø6.2) for anti-rotation of prosthesis.
- > Connected with the Abutment Screw (ILHS100).
- > Tightened with the 1.2 Hex Ratchet Driver and Torque Wrench.
- > Tightening torque force: 30N.cm.
- > Use the Scanbody for digital workflow.
- > Fixture level impression.


Hybrid L Ti-Base



Type	Octa		N-Octa	
Platform [Fixture Dia.]	Ø4.8 [Ø3.5 / Ø4.0 / Ø4.5]	Ø5.9 [Ø5.0 / Ø6.0]	Ø4.8 [Ø3.5 / Ø4.0 / Ø4.5]	Ø5.9 [Ø5.0 / Ø6.0]
Diameter	Ø5.1	Ø6.2	Ø5.1	Ø6.2
Length	5.5	5.5	5.5	5.5
Cuff				
0.8	ILO4815	ILO5915	ILN4815	ILN5915
2	ILO4825	ILO5925	ILN4825	ILN5925
3	ILO4835	ILO5935	ILN4835	ILN5935

- > Packing unit: 1 Hybrid L Ti-Base + 1 Abutment Screw.
- > For Screw-Cement or Cement Retained Abutment.
- > Titanium base for the strength of CAD/CAM customized abutment or crown.
- > Gold color for more translucent restoration.
- > Library available for EXOCAD®, 3Shape® & others.
- > Cutting surface (Ø5.1) and humped design (Ø6.2) for anti-rotation of the prosthesis.
- > Connected with the Abutment Screw (ILHS100).
- > Tightened with the 1.2 Hex Ratchet Driver and Torque Wrench.
- > Tightening torque force: 30N.cm.
- > Use the Scanbody for digital workflow.
- > Fixture level impression.

Scanbody



Type	Octa(Short)	Octa(Long)
Platform [Fixture Dia.]	Ø4.8 & Ø5.9 [Ø3.5 / Ø4.0 / Ø4.5 / Ø5.0 / Ø6.0]	Ø4.8 & Ø5.9 [Ø3.5 / Ø4.0 / Ø4.5 / Ø5.0 / Ø6.0]
Diameter	Ø4.5	Ø4.5
Height	6	10
	ISB406	ISB410

- > Packing unit: 1 Scanbody + 1 Abutment Screw.
- > For both, model-scanner and intra-oral scanner.
- > Made of 100% titanium alloy with a special coating applied.
- > No need to spray.
- > Connected with the Abutment Screw (ISHR110).
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 12~15N.cm.


Digital Analog



Platform [Fixture Dia.]	Ø4.8 [Ø3.5 / Ø4.0 / Ø4.5]	Ø5.9 [Ø5.0 / Ø6.0]
Diameter	Ø4.8	Ø5.9
Height	13.5	13.5
	IDR001R	IDR001W

- > Packing unit: 1 Digital Analog.
- > Analog of fixture for the working cast.
- > Used for both 3D printed model (RP) and stone model.
- > Select according to fixture platform.

Pick-up Impression Coping



Type	Octa	
Platform [Fixture Dia.]	Ø4.8 [Ø3.5 / Ø4.0 / Ø4.5]	Ø5.9 [Ø5.0 / Ø6.0]
Diameter	Ø5.5	Ø6.6
Length	13.7	13.7
	IIOR001	IOW001

- > Packing unit: 1 Pick-up Impression Coping + 1 Guide Pin.
- > For open tray impression.
- > Connected with the Guide Pin (IIOR001S).
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 12~15N.cm.


Abutment Screw



Diameter	Ø2.3
Height	8.6
	ILHS100

- > Packing unit: 1 Abutment Screw.
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 30N.cm.

Transfer Post



Type	Octa		N-Octa	
Platform [Fixture Dia.]	Ø4.8 [Ø3.5 / Ø4.0 / Ø4.5]	Ø5.9 [Ø5.0 / Ø6.0]	Ø4.8 [Ø3.5 / Ø4.0 / Ø4.5]	Ø5.9 [Ø5.0 / Ø6.0]
Diameter	Ø4.8	Ø5.9	Ø4.8	Ø5.9
Length	11.6	11.6	11.6	11.6
	ITOR400	ITOW500	ITNR400	ITNW500

- > Packing unit: Octa - 1 Transfer Post + 1 Guide Pin / N-Octa - 1 Transfer Post (Solid Type).
- > For closed tray impression.
- > Connected with the Guide Pin (Regular: ITOR400S / Wide: ITOW500S).
- > Tightened with the 1.2 Hex Driver and Torque Wrench.
- > Tightening torque force: 12~15N.cm.

COWELL® EXPERT INSTRUMENTS

An Expert knows what makes the results



MFS Kit (Multi-Functional Sinus™ Kit)

Designed to perform maxillary sinus lifting. Aqua Membrane Lifter, Drill designs, and Stopper System prevent perforation of sinus membrane. The kit includes all the instruments required for both crestal and lateral approach.

Easy Sinus Lift Kit

This revolutionary kit contains US Patented Modified Tap Drills and Spreaders in order to allow any dentists to easily lift, split or condense surrounding bone with simple drilling. Dentists can expect more predictable results, and patients can enjoy less traumatic surgeries with shorter chair time.

MFR Kit (Multi-Functional Removal™ Kit)

An ideal solution for fixture, abutment, and screw removal without trauma and bone loss.

InnoGenic® GBR Kit

An all-in-one solution for various types of GBR procedures.

InnoGenic® Autobone Harvester

Devised to harvest autogenous bone not only from the general site but also from the site where the implant will be placed. More than 1cc of bone chips can be harvested within 10 seconds.

COWELL® BMP Trepine Kit

An easy-to-use kit with drills and instruments for block-type bone collection, failed fixture removal, crestal & window approach for sinus lift, and bone chip extraction.

Atraumatic Extraction Kit

Used for the immediate and effortless extraction of the root of the tooth with simple procedures.

Direct Surgical Guide Kit




Used for flapless surgery, It can also serve as a guide for positioning the drill while measuring the thickness of the buccal bone, thereby preventing bone resorption and reducing the burden on the patient.

AO4 Surgical Stent

An excellent guide template to place implant precisely, especially for AO4 or AO6 technique.


Volume-up™ Guide System

Devised for preventing food penetration and forming natural cervical area by restoring contracted buccal alveolar bone & gingiva to the original shape and width.



Multi-Functional Sinus™ Kit
MFS KIT [KSA004]

> A comprehensive kit to approach direct & indirect maxillary sinus lift simply.



Aqua Ratchet Connector




Aqua Syringe Connector




Bone Carrier




Aqua Tube



Sinus Elevator



Aqua Lifter Silicon




Crestal Approach - Components

1. Point Drill 800~1,000rpm

- > Use to mark the point of perforation on cortical bone.
- > In the case of the remaining bone height is as low as 3.5mm, pay more attention when drilling.



Code KPD01S




2. 2.2 Twist Drill 800~1,000rpm

- > Use for making guide hole before using the Crestal Drill.
- > Connect the Crestal Drill Stopper according to the height of the remaining bone.



Code KSTD22






3. Crestal Drill 400~800rpm

- > Use the Crestal Drill sequentially according to the diameter of the fixture to be placed.
- > Can also be used if sinus floor is flat, incline, septum.
- > The Crestal Drill can be used about 50 times (depending on bone quality).




Fixture Dia.	Ø3.3	Ø3.5	Ø4.0	Ø4.5 / Ø5.0
Diameter	Ø2.8	Ø3.3	Ø3.7	Ø4.2
	KSCD28	KSCD33	KSCD37	KSCD42



※ Flat floor edges minimize damage to membrane.

4. Crestal Drill Stopper

- > Connected with a stopper to be drilled to the same length of the cartilage height of maxillary sinus which is measured by CT.
- > If not equipped with CT, fasten the stopper one step lower than expected and gradually increase the length.




Drilling Depth	1mm	2mm	3mm	4mm	5mm	6mm
	KSDS01	KSDS02	KSDS03	KSDS04	KSDS05	KSDS06


Drilling Depth	7mm	8mm	9mm	10mm	11mm	12mm
	KSDS07	KSDS08	KSDS09	KSDS10	KSDS11	KSDS12

5. Depth Gauge

- > Measure thickness of the residual bone after checking the perforation of the cartilage of the maxillary sinus (do not open completely, only the entrance side should be opened).
- > The stopper is attached to the base of the residual bone to separate the cartilage and membrane from the maxillary sinus.





Code KDG001S




6. Aqua Membrane Lifter System

- > After confirming that elevation of the cartilage of maxillary sinus, elevate membrane with the Aqua Membrane Lifter System.

- 1 Connect the Aqua Lifter to the Guide Holder.
- 2 Connect the Aqua Tube to syringe using the Aqua Syringe Connector (SC).
- 3 Inject saline solution equal to the amount of bone graft material to be used for syringe.
- 4 Tube connection to the Aqua Lifter Drill using the Aqua Ratchet Connector (RC).
- 5 Inject saline solution.




7. Torque Wrench



Code KTW001

8. Bone Carrier


> Insert bone graft material using the Bone Carrier.



※ If you need to expand hole, drill 1mm deeper using the crestal drill.

9. Bone Condenser


> After connecting the stopper with the Bone Condenser, elevate bone graft materials to inside of maxillary sinus.
> Rotate bone graft material using the Bone Condenser to disperse bone graft material (possible to do with the Depth Gauge).



※ If you need to expand hole, drill 1mm deeper using the crestal drill.


10. Implant Drill (Final)

> Drill 1~2mm more deeply than steps of the Crestal Drill.



11. Implant Placement

> If the residual bone is less than 3mm, do not implant the fixture, but bone graft only.




Crestal Approach - Drilling Sequence

> Placing implant over Ø4.0 is highly recommended.

1. Ø3.3 Narrow Fixture




2. Ø3.5 Fixture



3. Ø4.0 Fixture



4. Ø4.5 Fixture



※ Ø5.0 Fixture Normal Bone : Drilling with the Final Drill before placing implants are required.

※ Use a Drill that is one step shorter than the implant (E.g. 10mm implant, 8~9mm Drill).


Lateral Approach - Components

1. Ø6 Lateral Reamer 800~1,000rpm

- > Drill after fastening the stopper according to the height of the bone.
- > Round shape to prevent membrane perforation.



Code KSLD60




2. Ø6 Lateral Round Drill 800~1,000rpm


- > Drill after fastening the stopper according to the height of the bone.
- > Round shaped edge.
- > The residual bone should be replaced in the original position after drilling, sinus lifting & augmentation.



Code KSLRD60



3. Lateral Stopper




Drilling Depth	0.5mm	1mm	1.5mm	2mm	2.5mm	3mm
	KSDSL05	KSDSL10	KSDSL15	KSDSL20	KSDSL25	KSDSL30

4. Sinus Elevator

- > CSE-01 : Initial elevation of sinus membrane.




Code KSSE01



- > CSE-02 : as stepwise, after using CSE-01, used for elevation of sinus membrane.




Code KSSE02



- > CSE-03 : as stepwise, after using CSE-02, used for elevation of sinus membrane.



Code KSSE03




5. Ø4 Side Cutter 800~1,000rpm


- > When you expand window, must be connected with Stopper.




Code KSC60




6. Sinus Bone Graft



7. Implant Drill (Final)




8. Implant Placement



Easy Sinus Lift Kit [KSA001]


> Easy Sinus Lift Kit is the world's most innovative kit for performing maxillary sinus lift, ridge splits, and bone condensing cases. This revolutionary kit contains US Patented modified Tap Drills and Spreaders in order to allow any dentists to easily lift, split, or condense surrounding bone with simple drilling. Dentists can expect more predictable results, and patients can enjoy less traumatic surgeries with shorter chair time.



For All Surgery

> Universally used Drills / used for both sinus lift or ridge split.
> Drilling must be accompanied with copious amounts of refrigerated sterile irrigation.

Drill Speed : 800-2,000 rpm




For manual operation using Torque Wrench, Adapter needs to be connected with Machine Driver.

Sinus Lift

> Used in any maxillary sinus implantation.

Drill Speed : 20-30 rpm
Torque : 45 N.cm




Drill Speed : 100-500 rpm
Torque : 45 N-cm

Spreader

> Used in bone condensing or ridge split implantation.
> Also used in maxillary sinus lift & immediate placement cases.


Drill Speed : 20-30 rpm
Torque : 45 N.cm




Sinus Lift

• Tap Drill (Ø3.6, Ø4.6)

> The Tap Drill uses low speed and high torque to grind through the maxillary bone, and safely elevates sinus without membrane perforation.
> Must be used at 20~30 rpm / 45 N.cm.
> No irrigation is required.




Diameter	Ø3.6	Ø4.6
	KMTD36S	KMTD46S




• Twist Drill (Ø3.6, Ø4.6)

> The Twist Drill is used after tapping as final drill for dense bone (bone quality 2 or greater) or to eliminate tapping thread in order to facilitate bone grafting.
> Must be used at 100~500 rpm / 45 N.cm.
> No irrigation is required.




Diameter	Ø3.6	Ø4.6
	KTWD36S	KTWD46S




Spreader

• Tap Drill (Ø3.2, Ø3.8, Ø4.2, Ø4.8, Ø5.1)

> The Spreader Drill is used to condense and/or spread the bone in either sinus lift or ridge split cases.
> Must be used at 20~30 rpm / 45 N.cm.
> No irrigation is required.




Diameter	Ø3.2	Ø3.8	Ø4.2	Ø4.8	Ø5.1
	KMTD32S	KMTD38S	KMTD42S	KMTD48S	KMTD51S

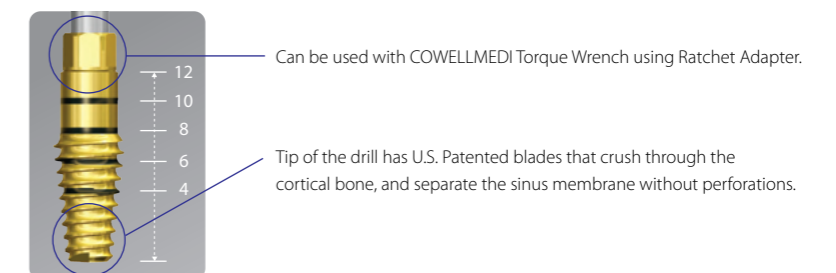


Sequence - Sinus Lift

• Only use of Sinus Lift Drill


1 Sinus Lift (Ø4.0 Fixture)




▶ Immediate Implantation and Sinus Lift Technique with Tap Drill (Ø4.0 Fixture)



2 Sinus Lift (Ø5.0 Fixture)




▶ Immediate Implantation and Sinus Lift Technique with Tap Drill (Ø5.0 Fixture)




• Recommend to use Sinus Lift Drill and Spreader Drill together

1 Sinus Lift (Ø4.0 Fixture)




2 Sinus Lift (Ø5.0 Fixture)

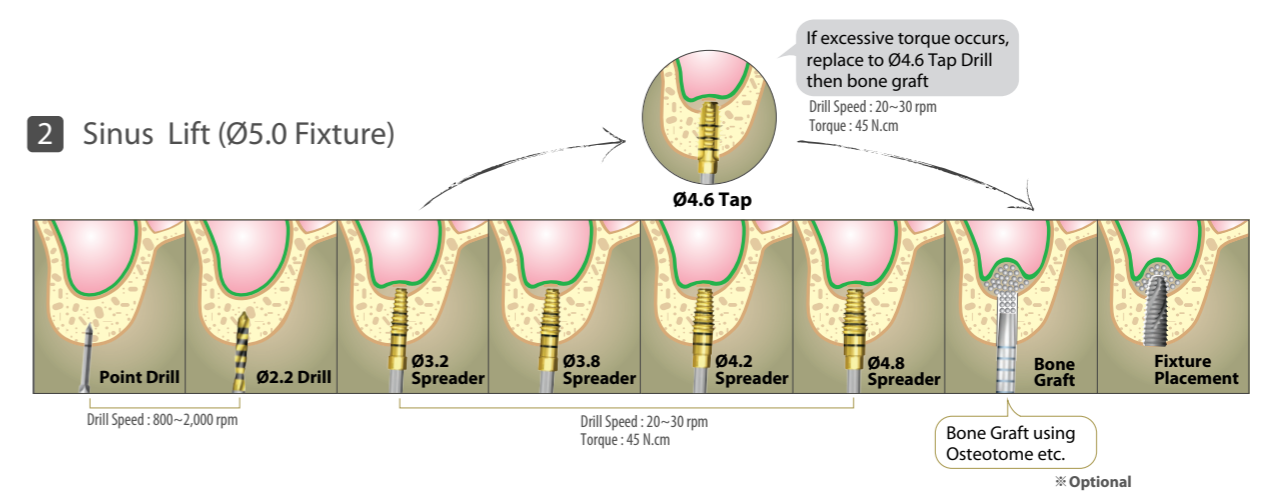


Note

- > Recommend to use Sinus Lift Drill and Spreader Drill together during the Sinus Lift operation.
- > Easily operate by using Ø3.2 Spreader rather than Point Drill.
- > Avoid to over press surrounding alveolar bone using Final Drill before fixture placement in D2.


ex) Ø4.0 Fixture placement



▶▶ Ridge Split and Block Bone Augmentation Technique with Spreader Drill (Ø4.0 Fixture)




Sequence - Spreader




Multi-Functional Removal™ Kit
MFR KIT [KHA001]


> Easy removal of fractured fixture / screw / abutment.

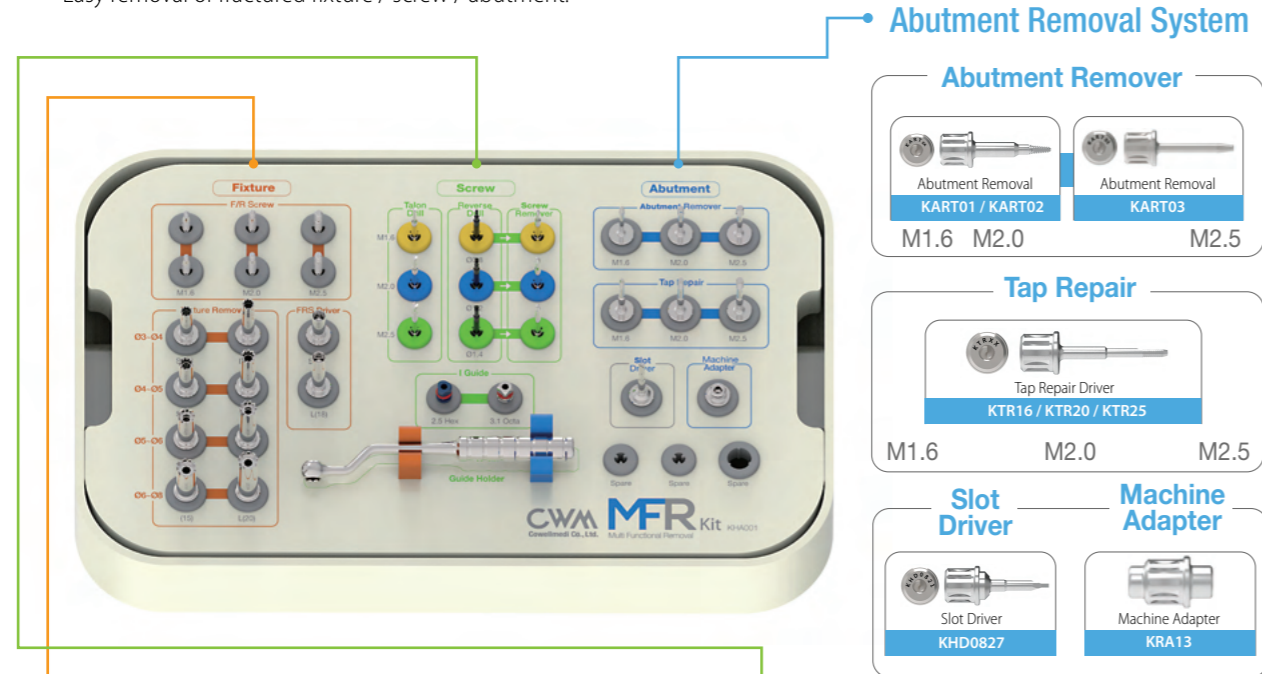

Fixture Removal System




Screw Removal System



MFR Kit - Components

1. Fixture Removal System

- 1 Connect the F/R Screw to the FRS Driver.
- 2 Connect the F/R Screw mounted FRS Driver to the fixture (clockwise 40~60N.cm) and remove the FRS Driver.
- 3 Connect the Fixture Remover to the F/R Screw (counterclockwise).
- 4 Remove the fixture after connecting the Torque Wrench (counterclockwise, 100~400N.cm).
- 5 To remove the fixture from the Fixture remover, use such device as vise to fix the Fixture Remover and connect to the Torque Wrench.
- 6 After connecting the FRS Driver to the F/R Screw, use the Torque Wrench to remove the F/R Screw (counterclockwise).




- ※ One-time use of the F/R Screw is recommended (bending or fracture may happen if more than 100N.cm and using twice may be possible if less than 100N.cm).
- ※ Sufficient irrigation is required when removing the fixture.
- ※ When the maximum torque is exceeded, the fixture may be bent or fractured.
- ※ If the fixture can not be removed even with maximum torque, remove the Fixture Remover & F/R Screw, remove bones around fixture using round bur and retry to remove.

2. Screw Removal System

Talon Drill

- 1 Check the broken screw size inside the fixture.
- 2 Connect the I Guide corresponding to the fixture to the Guide Holder and fasten to the fixture.
- 3 Insert the Talon Drill into the I Guide Hole.
- 4 Remove the screw by pressing force (counterclockwise, 60~80rpm).




- ※ If the I Guide and fixture could not be correctly connected, the path is not correct.

Reverse Drill & Screw Remover

If the screw could not be removed by the Talon Drill

- ① Form the hole on the fractured screw (depth 1~2mm / counterclockwise / 1,200~1,400rpm).
- ② Use the Screw Remover according to the created drill hole, remove the screw by pressing force (counterclockwise, 80N.cm).




- ※ If the path of the I Guide and fixture did not match, it would be difficult to remove the screw because the drill hole is away from the center of the screw.
- ※ Reverse drilling requires removal of chips by irrigation & suction.
- ※ The fractured screw may be removed during reverse drill hole creation.
- ※ If necessary, fasten to the Machine Adapter and use the hand or Torque Wrench.



3. Abutment Removal System


Abutment Remover

- ① Used when 2 piece type abutment is fractured.
- ② Connect to the Abutment Remover (clockwise).
- ③ Connect correctly and wiggle to left and right side.




Tap Repair

- ① Used when the thread inside the fixture is occluded and damaged.
- ② Reproduce the thread using the Tap Repair.

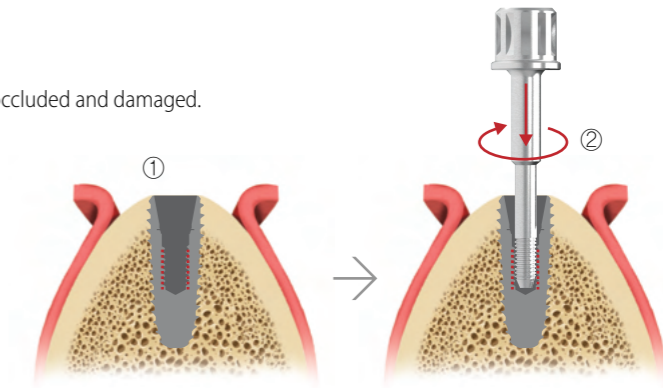

Slot Driver

- ① Used for damaged solid type abutments, healing abutments, and cover screws.
- ② Form a slot on the surface of the damaged abutment using a round bur.
- ③ Connect the Slot Driver to the formed slot and remove it (counterclockwise).



4. Torque Wrench



Place the fixture
(clockwise, 40~80N.cm).



Remove the fixture
(counterclockwise, 100~400N.cm).

InnoGenic® GBR Kit [KIGBR001]

> An all-in-one solution for various types of GBR procedures.

The length of the product can be measured with the scale marked on the middle tray of the kit.

Drill

- Fixing Screw Drill KFS010
- Tenting Screw Drill KTSD14

Drill Stopper

- 3mm KIGDS03
- 5mm KIGDS05
- 7mm KIGDS07

Driver

- Machine KFSMD24
- Handle KFSHD70
- Machine KTSM24
- Handle KTSHD70

Fixing

- Machine KFSMD24
- Handle KFSHD70

Tenting

- Machine KTSM24
- Handle KTSHD70

Harvesting Drill

- Round Bur KIGRB10
- Bone Trimmer KIGBT50
- Ø3.5 Drill KBH35
- Ø5.0 Drill KBH50
- 0.9 Hex Driver KHD0921
- Silicon Shield KBHDS01

Fix Connector F/Connector Fixture

- 0.5mm KIGFC4505
- 0.5mm KIGFC4505
- 1.0mm KIGFC4510
- 1.0mm KIGFC4510
- 1.5mm KIGFC4515
- 1.5mm KIGFC4515
- 2.0mm KIGFC4520
- 2.0mm KIGFC4520

Cover Cap C/Cap

- Ø4.5 KIGCC45
- Ø4.5(3mm) KIGHC453
- Ø4.5(3mm) KIGHC453
- Ø4.5(4mm) KIGHC454
- Ø4.5(4mm) KIGHC454
- Ø4.5 KIGCC45
- Ø5.5(3mm) KIGHC553
- Ø5.5(3mm) KIGHC553
- Ø5.5(4mm) KIGHC554
- Ø5.5(4mm) KIGHC554

Healing Cap H/Cap

- Ø4.5(3mm) KIGHC453
- Ø4.5(3mm) KIGHC453
- Ø4.5(4mm) KIGHC454
- Ø4.5(4mm) KIGHC454
- Ø5.5(3mm) KIGHC553
- Ø5.5(3mm) KIGHC553
- Ø5.5(4mm) KIGHC554
- Ø5.5(4mm) KIGHC554



Screw Kit KIGCS001

- Fixing Screw: 3mm (KIGFS03), 5mm (KIGFS05), 7mm (KIGFS07)
- Tenting Screw: 7mm (KIGTS07), 10mm (KIGTS10), 13mm (KIGTS13), 15mm (KIGTS15)
- Tenting Cap T/Cap: 0.3mm (KIGTC32), 0.3mm (KIGTC32), 0.3mm (KIGTC32)


















Scale: 0, 3, 5, 7, 10, 13, 15, 18, 20, 23, 25, 30

Screw Kit KIGICS001

- Used without removing the Screw Kit from the inside of the kit tray (Remove to use if necessary only).
- Made of special material for autoclaving.
- * Rotate the upper lid to take out the selected product.



Composition

Classification	Product	Code	Quantity	
Bone	Fixing Screw (Fixing)	 KIGFS03	5	
		 KIGFS05	5	
		 KIGFS07	5	
	Tenting Screw (Tenting)	 KIGTS07	4	
		 KIGTS10	4	
		 KIGTS13	4	
		 KIGTS15	4	
	Tenting Cap (T/Cap)	 KIGTC32	3	
	Fixture	Fix Connector (F/Connector)	 KIGFC4505	2
			 KIGFC4510	2
 KIGFC4515			2	
 KIGFC4520			2	
Cover Cap (C/Cap)		 KIGCC45	2	
Healing Cap (H/Cap)		 KIGHC453	2	
		 KIGHC454	2	
		 KIGHC553	2	
	 KIGHC554	2		

Empty Screw Kit KIGICS





Bone

Fixing Screw (Fixing)

- Used to fix the membrane to the bone.
- Place slowly using the Fixing Driver (Machine/Handle).
- 3, 5 and 7mm length can be selected according to the bone quality.
- In hard bone, use after forming a basic drill hole using the Fixing Screw Drill.
- The wedge-shaped design is advantageous for self-tapping, allowing it to be fixed without drilling in normal bone.
- The double thread shortens the placement time.

D(Ø,mm)	C(mm)	L(mm)	H(mm)	Code
2.0	0.6	3.0	3.6	KIGFS03
		5.0	5.6	KIGFS05
		7.0	7.6	KIGFS07





Bone

Tenting Screw (Tenting)

- Used when a large area of vertical / horizontal GBR is required.
- Leave space for bone grafts.
- Place slowly using the Tenting Screw Driver (Machine/Handle).
- Recommended placement depth : Hard bone-3mm, Normal bone-5mm, Soft bone-more than 5mm.
- Initial fixation of at least 15~25N.cm is required. Tightening more than 35N.cm may cause fracture of the Tenting Screw so it must be fixed below 35N.cm.
- In normal bone, it is recommended to form a hole at least 3mm deep using the Tenting Screw Drill before placing the Tenting Screw.
- The wedge-shaped design is advantageous for self tapping, allowing it to be used without drilling in normal bone.
- The double thread shortens the placement time.
- Use the Tenting Cap if necessary.

D(Ø,mm)	C(mm)	L(mm)	H(mm)	Code
3.2	2.5	7.0	9.5	KIGTS07
		10.0	12.5	KIGTS10
		13.0	15.5	KIGTS13
		15.0	17.5	KIGTS15




Bone

Tenting Cap (T/Cap)

- Used to fix membrane on the Tenting Screw.
- Tightened with the 0.9 Hex Driver.
- Recommended tightening torque force : 5~8N.cm.

D(Ø,mm)	C(mm)	L(mm)	H(mm)	Code
3.2	0.3	2.8	3.1	KIGTC32




Fixture

Cover Cap (C/Cap)

- Used to fix membrane over the Fix Connector.
- For submerged surgery in case of sufficient soft tissue.
- Tightened with the 0.9 Hex Driver.
- Recommended tightening torque force: 5~8N.cm.

D(Ø,mm)	C(mm)	L(mm)	H(mm)	Code
4.5	0.3	3.4	3.7	KIGCC45




Fixture

Fix Connector (F/Connector)

- Used to fix the membrane along with the Cover Cap or Healing Cap after connecting to the fixture.
- Tightened with the 0.9 Hex Driver.
- Recommended tightening torque force: 12~15N.cm.
- Available for the INNO Submerged, Submerged Short Fixtures and other fixtures compatible with them only.

D(Ø,mm)	C(mm)	L(mm)	H(mm)	Code
4.5	0.5	5.7	6.2	KIGFC4505
	1.0		6.7	KIGFC4510
	1.5		7.2	KIGFC4515
	2.0		7.7	KIGFC4520




Fixture

Healing Cap (H/Cap)

- Used to fix membrane over the Fix Connector.
- For non-submerged surgery in case of insufficient soft tissue.
- Connect by using the 0.9 Hex Driver.
- Recommended tightening torque force: 5~8N.cm.


D(Ø,mm)	C(mm)	L(mm)	H(mm)	Code
4.5	3.0	3.4	6.4	KIGHC453
	4.0		7.4	KIGHC454
5.5	3.0		6.4	KIGHC553
	4.0		7.4	KIGHC554



Fixing Screw Drill & Tenting Screw Drill


- Used to place the Fixing Screw / Tenting Screw mainly in hard bone.
- Also used to perforate cortical bone when blood supply is required.
- For normal bone, drill only 3mm deep if necessary.
- Drill before placing the Fixing Screw / Tenting Screw.
- Laser-marked at 3, 5, and 7mm long from the tip of the drill and the length can be controllable using the Drill Stoppers.
- Color-banded for distinction (Red : Fixing Screw Drill, Blue : Tenting Screw Drill).
- Recommended drilling speed : 1,000~1,200rpm.

Classification	D(Ø,mm)	L(mm)	H(mm)	Code
Fixing Screw Drill	1.0	10	31.5	KFSD10
Tenting Screw Drill	1.4			KTSD14




Drill Stopper

- Used by connecting to the Fixing Screw Drill / Tenting Screw Drill.
- 3mm : Yellow, 5mm : Red, 7mm : Blue



Classification	D(Ø,mm)	H(mm)	Code
3mm	3.5	13.5	KIGDS03
5mm		11.5	KIGDS05
7mm		9.5	KIGDS07




0.9 Hex Driver (Ratchet)

- Used to install the Tenting Cap, Fix Connector, Cover Cap and Healing Cap.

D(Ø,mm)	L(mm)	H(mm)	Code
1.2	8	15	*KHD0915
	14	21	KHD0921
	20	27	*KHD0927



* Optional



Fixing Screw Driver & Tenting Screw Driver (Machine)



- Used to place the Fixing Screw / Tenting Screw using Contra-angle.
- Color-banded for distinction (Red : Fixing Screw Driver, Blue : Tenting Screw Driver).

Classification	D(Ø,mm)	L(mm)	H(mm)	Code
Fixing Screw Driver	1.6	6.0	24.0	KFSMD24
Tenting Screw Driver	2.2			KTSM24



Fixing Screw Driver & Tenting Screw Driver (Handle)


- Used to place the Fixing Screw / Tenting Screw using the Driver Handle.
- Color-banded for distinction (Red : Fixing Screw Driver, Blue : Tenting Screw Driver).




Classification	D(Ø,mm)	L(mm)	H(mm)	Code
Fixing Screw Driver	1.6	6.0	70.0	KFSHD70
Tenting Screw Driver	2.2			KTSHD70

Driver Handle

- Used to place and remove the Fixing Screw / Tenting Screw by connecting the Driver Handle.




D(Ø,mm)	L(mm)	H(mm)	Code
19.8	75	135.0	KIGH




Round Bur

- Used to perforate cortical bone when blood supply is required.
- Recommended drilling speed : 1,200~1,500rpm.




D(Ø,mm)	L(mm)	H(mm)	Code
1.0	9.5	34.0	KIGRB10




Bone Trimmer

- Used to perform osteoplasty on the outer wall of remaining bone all during GBR and to flat the bone surface for improving the fit of membrane.
- Used to remove remaining granulation tissue of bone defect part (use instead of surgical curette).
- Recommended drilling speed : 1,200~1,500rpm.



D(Ø,mm)	L(mm)	H(mm)	Code
5.0	13	34.0	KIGBT50




Harvesting Drill & Drill Stopper

- Drill for convenient harvesting of autogenous bone in the form of bone chip in a short period of time.
- The Silicon Shield of the Ø3.5 Harvesting Drill makes sure with no bone chip loss while drilling (Bone chip can be collected at implant site).
- 6 Silicon Shields are included in the Kit (1 is assembled with the Ø3.5 Harvesting Drill and 5 are packed in the lower tray).
- The maximum drilling depth of the Ø3.5 Harvesting Drill is 12mm, so it needs to be drilled slowly.
- Remove while rotating the drill.
- Recommended drilling speed : 300~500rpm.

D(Ø,mm)	L(mm)	H(mm)	Code
3.5	9.5	39.2	KBH35
5.0	6.5	36.5	KBH50


Drill Stopper	D(Ø,mm)	H(mm)	Code
	5.6	9	KBHD3540
6	14.3	KBHD4550	



* For the details of InnoGenic® Autogene Harvester, refer the pages 218~222.

Bone Carrier

- Narrow tip is beneficially handled in most of the bone graft techniques.
- Bone graft particles can be accurately and safely injected without contamination.
- rhBMP-2 can be easily coated to the implant due to circular groove of tip.
- Bone graft particles and rhBMP-2 solution can be well mixed on the circular groove.



Bone Carrier	D(Ø,mm)	H(mm)	Code
	6	94	KBBC01

* Bone Carrier length is 94mm and the total length after stretching is 114mm.




InnoGenic® Autobone Harvester [KIAH001]

> Maximize Your Return On Minimal Investment, Guaranteed!



Harvesting Drill



Drill Stopper



Silicon Shield




* 1EA assembled with the Drill Stopper (KBHD3540).
5EA placed in the lower tray.

Key Concepts

Maximize your return on minimal investment

The key concept of the Autobone Harvester Plus is to harvest a large amount of the autogenous bone chips from the implant site that can be wasted into the suction during implant drilling procedure.

Features: Drill



Features: Stopper & Silicon Shield

For Ø3.5 & 4.0 Drill



Stopper


Used by fastening to the Stopper Holder of Ø3.5 & 4.0 Drill.

+



Silicon Shield (*Exclusive for Ø3.5 & 4.0)

- Used by fastening to Ø3.5 & 4.0 stopper.
- Prevents deviation of bone chips.
- Allows bone chip harvesting from the implant site.
- Reusable transparent silicon material allows checking drilling position and bone chips being harvested.



Shield


The lip-shaped shield is brought into close contact with the bone and makes sure with no bone chip loss while drilling.

For Ø4.5 & 5.0 Drill



Stopper

Used by fastening to the Stopper Holder of Ø4.5 & 5.0 Drill.




Drilling Depth : 5mm

For 6.0 Drill



Stopper

Used by fastening to the Stopper Holder of Ø6.0 Drill.



Harvesting sequence:

Implant Site using Ø3.5/4.0

Harvesting Drill with the Silicon Shield



• Point drill to mark harvesting and implant site.



• Select Ø3.5/4.0 Drill and insert the Stopper into the selected Drill. And put the Shield on the Ø3.5&4.0 Stopper.



• Drill at 300 to 500rpm with irrigation and harvest bone chips.



• Disassemble the Silicon Shield, the Stopper and collect the bone chips for bone grafting.



• Use Final Drill (equal to or over Ø3.5/4.0) according to the drilling protocol of the manufacturer and treatment planning.




• Place the implant.



• Apply the harvested bone chips on the site.

Harvesting sequence: Buccal Bone Harvesting using Ø3.5/4.0/4.5/5.0/6.0 Harvesting Drill

Select the drill according to its diameter and clinical indications.



• Drill at 300 to 500rpm with irrigation and harvest autogenous bone chips.

• Apply the harvested bone chips on the site.

A Clinical Case using Ø3.5/4.0 Harvesting Drill

by Dr. Soohong Kim, DDS, Ph.D



Drilling at 300rpm with irrigation was carried out after marking implant and harvesting position.



The Silicone Shield was brought into close contact with various types of bone levels and prevented bone chip loss.



The amount of bone taken was easily ascertained, through the transparent Silicone Shield.



The bone was transferred to a bone dish after disassembling the Silicon Shield and Stopper. The amount of the bone was much more than expected.




After the implant placement, healing abutments were connected and carried out GBR in the defective area.

* 2 Step Harvesting : Drilling to 7mm is recommended after transferring bone chips to bowl since the Stopper & Silicon Shield are fully filled with bone chips while 4mm drilling.


COWELL® BMP Trepine Kit [KBT001]

> An easy-to-use kit with drills and instruments for block-type bone collection, failed fixture removal, crestal & window approach for sinus lift and bone chip extraction.



Trepine Drill I: Block Bone Extraction

Guide & Block Bone Trepine Drill



Trepine Drill II: Failed Fixture Removal

Fixture Removal




Trepine Drill III: Window Opening for Lateral Window Approach

Window Trepine



Implant Site Drill: Sinus Lift & Bone Chip Extraction Prior to Implant Placement

Implant Site



Product	Diameter	Code
Block Bone Guide Drill	Ø 6.0 (Inner)	KBGT60
	Ø 7.0 (Inner)	KBGT70
	Ø 8.0 (Inner)	KBGT80
Block Bone Trepine Drill	Ø 6.0 (Inner)	KBT60
	Ø 7.0 (Inner)	KBT70
	Ø 8.0 (Inner)	KBT80
Fixture Removal Trepine Drill	Ø 4.2 (Inner)	KFRT40
	Ø 4.7 (Inner)	KFRT45
	Ø 5.2 (Inner)	KFRT50
Window Trepine Drill	Ø 7.0 (Outer)	KWTT60
Implant Site Drill	Ø 3.5 (Fixture)	KTIS35
	Ø 4.0 (Fixture)	KTIS40
	Ø 4.5 (Fixture)	KTIS45
	Ø 5.0 (Fixture)	KTIS50

Trephine Drill I Block Bone Extraction

This Drill allows the collection of block-type autogenous bone with a required size in the case of regenerating a wide bone defect and severe bone resorption.

Block Bone Guide


- > This guide helps the target block bone to be accurately positioned and the Trephine Drill to be stably engaged with the bone.
- > Desired rpm: 800~1,000rpm.

Block Bone Trephine Drill

- > This drill is engaged with the bone groove with the help of the block bone guide to collect the block bone with a desired size.
- > Desired rpm: 800~1,000rpm.

Diameter	Ø 6.0 (Inner)	Ø 7.0 (Inner)	Ø 8.0 (Inner)
	KBGT60	KBGT70	KBGT80

Diameter	Ø 6.0 (Inner)	Ø 7.0 (Inner)	Ø 8.0 (Inner)
	KBT60	KBT70	KBT80




Trephine Drill II Failed Fixture Removal

Diameter	Ø 4.2 (Inner)	Ø 4.7 (Inner)	Ø 5.2 (Inner)
	KFRT40	KFRT45	KFRT50

Trephine Drill III Window Opening for Lateral Window Approach


Diameter	Ø 7.0 (Outer)
	KWTT60



Implant Site Drill Sinus Lift & Bone Chip Extraction Prior to Implant Placement


Diameter	Ø 3.5	Ø 4.0	Ø 4.5	Ø 5.0
	KTIS35	KTIS40	KTIS45	KTIS50

- > Used before the Final Drill is used (simplified drilling sequence).
- > Advantageous for securing autogenous bone.
- > Less rpm drilling leads to low bone heating.
- > Also used as a sinus lift tool (Sinus Lift).
- > Desired rpm : 20~30rpm.



Atraumatic Extraction Kit [KAE001]

> Used for the immediate and effortless extraction of the root of the tooth with simple procedures.



(1) Diversity

A root extraction can be done regardless of whether residual amount of root is large or small.

(2) Safety

A root extraction without the risk of damaging adjacent teeth is possible using the Rest Plate, Elevator, etc.


(3) Convenience

A very simple and convenient root extraction is possible, compared to the existing extraction method.

(4) Reduced Procedure Time

The procedure time is reduced due to the simple procedure.

Composition



1. Extraction Drill


> The Extraction Drill is composed of three types of Drills (Ø1.3 / Ø1.7 / Ø2.1) that can be selected according to the case.

Ø1.3 Drill




Code KAAD13

Ø1.7 Drill



Code KARD17

Ø2.1 Drill




Code KAMD21

2. Extraction Screw

> The Extraction Screw is fastened into the hole that was created by the Extraction Drill via the Screw method, and it is stably fixed to the remaining root. It is composed of the Ø1.8 / Ø2.2 / Ø2.6 Screws that can be selected according to the Extraction Drill.


> The Ø1.8 Screw is used for vital root of which canal is not treated, after using the Ø1.7 Drill.

Ø1.8 Screw




Code	KAAS16	* KAAS16X
Length	10	15

* Extra product




Ø2.2 Screw




Code	KARS20	* KARS20X
Length	10	15

* Extra product



Ø2.6 Screw



Code KAMS25




3. Post Driver

> After connecting the Post Driver to the Extraction Screw, turn the Torque Wrench in a clockwise direction in order to fix it to the hole that was created by the Extraction Drill (recommended torque : Min. 20N.cm ~ Max. 35N.cm).



4. Rest Plate


> The Rest Plate is connected between the Extraction Screw and the Torque Head. It protects the part with silicon that comes into direct contact with the adjacent teeth in order to prevent teeth damage. It also serves as a support for the Elevator and Torque Wrench.



5. Torque Head


> The Torque Head is connected to the Extraction Screw that is fixed in the tooth to be extracted. It fixes the gap of the Rest Plate and it can be used with the Elevator.

> If the root to be extracted has both distal and mesial adjacent teeth, it will be extracted with the Torque Wrench (recommended torque : 100N.cm or less).



6. Elevator

> The Elevator is used by connecting it with the Torque Head and extracting the root by applying force toward a distal or mesial direction.



How to Use


1. Extraction Drill

Create a hole on the tooth to be extracted using the Extraction Drill.



Caution A

- The Extraction Drill must follow the neural root canal during drilling.
- Drill down to at least 10mm because extraction is possible even if the Drill and Screw penetrate the root.



2. Extraction Screw

Connect the Extraction Screw to the Post Driver and fix it to the hole created by rotating it clockwise (recommended torque: Min. 20N.cm ~ Max. 35N.cm).




Caution B

- Drill to a depth of 10~12mm and insert the Extraction Screw at a depth of 10mm.
- Fix the Screw with 20~25N.cm.


Connect Post Driver to the Extraction Screw.

* Drilling Sequence

Root Canal Preparation



Atraumatic Extraction kit




Caution C

- Fix the screw with a torque of 20~25N.cm. If it is not applied, use a thicker Screw.
- The low torque force causes the Screw to fall out during the extraction, and the over torque force fractures tooth root.

3. Rest Plate

After removing the Post Driver, connect a Rest Plate to the Extraction Screw by taking into account the adjacent teeth.



Rest Plate

4. Torque Head


Connect the Torque Head to the Extraction Screw projected above the Rest Plate by rotating it clockwise.



Connect Torque Head to Screw

5. Torque Wrench

Extract the tooth by rotating the Torque Head clockwise using the Torque Wrench.




Extraction Root

Caution D

- Extraction using the Torque Wrench is possible in a root with mesiodistal root.

Caution E

- If there are adjacent teeth with 2 or higher swaying degrees, upward pulling or downward pressing should be applied using the Elevator so that the teeth will not receive force during extraction.



Caution F

- If there is an adjacent tooth projected to the mesiodistal root, it must be extracted using the Elevator.

Direct Surgical Guide Kit [KDSG002]

- > Used for flapless surgery, flapless.
- > Served as a guide for positioning the drill while measuring the thickness of the buccal bone, thereby preventing bone resorption and reducing the burden on the patient.
- > Stable drill positions can be guided to various cases by combining different surgical instruments (E.g., Position Guide, Linker, and Width Guide).



(1) Safety

Safe operation is possible by measuring the thickness of the buccal bone in order to prevent buccal bone resorption.

(2) Reduced Pain


It is possible to minimize the burden on the patient by reducing the pain and swelling from a flapless surgery without going through the incision step that is carried out during the general implant surgery.


(3) Accuracy and Diversity

An accurate operation is possible depending on the bone width and implant diameter by combining the operation instruments (E.g., Linker, Position Guide, and Width Guide). It can be used for various cases, such as single, bridge, etc.


1. Buccal Position Guide

- > Use the depth pin positioned at the bottom of the guide according to the bone width and fixture diameter. This will enable you to maintain the buccal bone thickness of the implant. The guide should be connected to the guide holder.
- > The length can be distinguished with the O-ring color of the post.
- > Be careful in using the depth pin because it is extremely sharp.






Caution A Please fix the depth pin of the Buccal Position Guide to the buccal bone surface 5mm below the gingiva or the alveolar crest.




Caution B In a defective buccal bone or a thin buccal bone due to tooth extraction, fix the depth pin of the Buccal Position Guide to the surface 5mm below the gingival or the alveolar crest, from the lingual or palatal side.

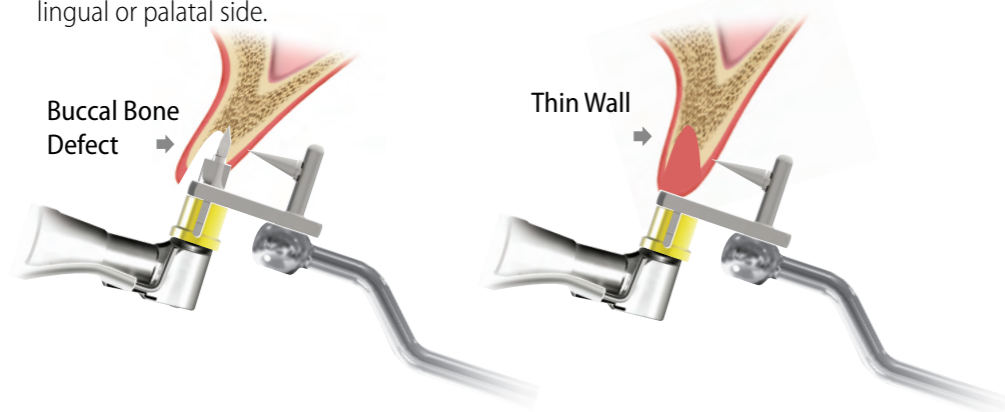

Caution C Select the 1, 2, or 3mm Buccal Position Guide depending on the alveolar bone width and implant diameter to determine the buccal bone thickness.

Bucco-palatal bone width




Fixture diameter




Black O-Ring
Under 7mm bone width,
under Ø4.0mm fixture

Bucco-palatal bone width




Fixture diameter




Red O-Ring
Bone Width 7~9mm,
Ø4.0mm~Ø4.5mm fixture

Bucco-palatal bone width




Fixture diameter




Blue O-Ring
Over 9mm Bone Width,
Ø5mm fixture

2. Width Guide

> Select the 7, 8, 9, or 10mm-width guide according to the implant crown diameter, mount it on the Buccal Position Guide, and Drill the center of the implant (the size is distinguished by color).




The width guide is used by connecting it with the sleeve of the Buccal Position Guide.




Buccal Position Guide

How to use according to the mesiodistal dimension-1
(Use of the Buccal Position Guide)




Mandible	Central incisor	Lateral incisor
Mesiodistal dimension	5.4	6.0

How to use according to the mesiodistal dimension-2
(Use of the combined Width Guides)

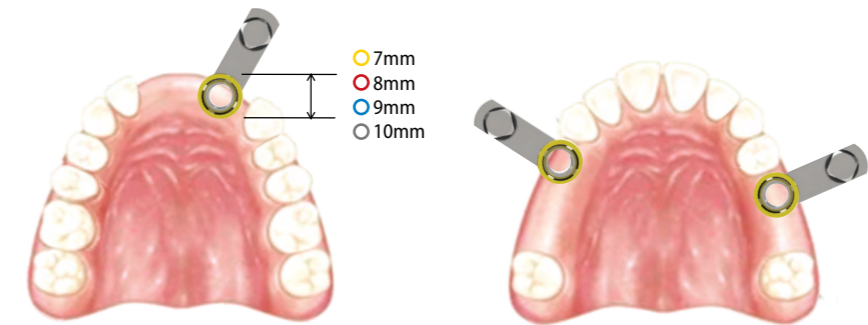

Maxilla	Lat. Incisor	1 st Premolar	2 nd Premolar
Mesiodistal dimension	7.3	7.7	7.3




Mandible	Canine	1 st Premolar	2 nd Premolar
Mesiodistal dimension	7.2	7.3	7.3



Maxilla	Central Incisor	Canine	1 st Molar	2 nd Molar	Mandible	1 st Molar	2 nd Molar
Mesiodistal dimension	9.2	8.3	10.5	9.5	Mesiodistal dimension	11	10

3. Position Guide


- > Guide the Drill position according to the distance between implant centerlines (7, 9, 11mm).
The device consists of three gaps : 3mm, 5mm, and 7mm from the Ø4mm fixture interface.
- > In continuous implants, select the 7, 9, or 11mm Position Guide according to the crown size, and mount it on the Buccal Position Guide to drill.



*The Position Guide must be used in combination with the Buccal Position Guide and linker.
It cannot guide the Drill position accurately when used alone.


Application of the 7mm Position Guide

(when the mesiodistal distance between the two missing teeth is at least 14mm)




Application of the 9mm Position Guide

(when the mesiodistal distance between the two missing teeth are at least 16mm)




Application of the 11mm Position Guide

(when the mesiodistal distance between the two missing teeth are at least 18mm)



4. Linker

- > When you perform prosthesis with a bridge in a continuous implant, connect the 11mm Linker to the position guide and the Buccal Position Guide to drill.



Assembly


- ① Position Guide + Linker
- ② Position Guide + Linker + Buccal Position Guide

① The Linker is connected to the Position Guide by setting the linker sleeve in a downward position.


② After connecting the Linker by setting the sleeve of the Buccal Position Guide in a downward position, it can be used by adjusting it according to the mesiodistal distance.

5. Point / Crestal Cutter Drill

- > A hole is created on the cortical bone in order to facilitate the Initial Drill.
- > The gingiva residue is removed while flattening the uneven alveolar bone surface.



Buccal Position Guide Assembly



* After connecting the guide handle to the buccal position guide, fix it at the site where the implant will be placed and insert the Point / Crestal Cutter Drill into the hole inside the Sleeve.


6. Guide Handle

- > The Guide Handle guides the position and direction by connecting it with the Buccal Position Guide.




Angulation of Guide assembly

1. Mesio-distal angle: parallel with adjacent tooth
2. Bucco-lingual angle



* The angle of the guide can be predicted according to the shape of the tooth.



Drilling Sequence (Flapless Surgery)



* Form basic holes with a crystal cutter. Then, select a drilling sequence according to the implant diameter.

AO4 Surgical Stent [KDSS001]

> Guide the position of Implant and Drill.




Characteristic

- > Guide the position of the implant and drill during implant placement.
- > It improves the stability and accuracy in surgery, and it can shorten the time.
- > By preventing the loss of healthy gums as much as possible, pre-fabricated prostheses can be placed immediately after surgery without the need for gum restoration.
- > Angled line allows more precise and predictable surgery.

Eligible for


- > A toothless patient.
- > Patient who do not want long-period of surgery.
- > Patients suffering from adult diseases such as hypertension and diabetes.
- > Patients who need precise implant treatment.

Instruction




Place the AO4 Surgical Stent

- Make an incision for flap lift.
- Place the AO4 Surgical Stent using Ø2mm Twist Drill.
* It is needed to check the position of mental foramen.



Place the INNO Fixture


- Drill with reference to the angled line and place the fixture.



Place the Multi S&A Abutment

- After placing the INNO fixture, connect the Multi S&A Abutment according to the site.
* Posterior site: Place the Multi A abutment (30°) with 30N.cm torque force.
* Anterior site: Place the Multi A abutment (15°) or the Multi S abutment with 15N.cm torque force (it is possible to allow emergence of the prosthetic screw).

or



Placement Lock Abutment


- After placing the INNO Fixture, connect Lock Abutment according to the site.
* If implant placement at an angle is not appropriate or not desired, using the INNO Sub. Short Implant is highly recommended.

Volume-up™ Guide System

> Devised for preventing food penetration and forming natural cervical area by restoring contracted buccal alveolar bone & gingiva to the original shape and width.

1. CONCEPT


• Peri-implant inflammations represent serious diseases after dental implant treatment, which affect both the surrounding hard and soft tissue.



To achieve long term success of implant without complications like peri-implantitis, right position of fixture with min. 2mm of buccal bone width for buccal gingival regeneration and alveolar bone regeneration at min. 3mm lower position to maintain gingival height is extremely essential.

Min. 2mm of buccal bone regeneration to maintain having buccal gingiva.
(Int J Periodontics Restorative Dent 2005)


Alveolar bone regeneration at minimum 3mm lower position to maintain gingival height.
(Clin Oral Implants Res 2000;11: 1-11.)



The Volume-up™ Guide System helps place implant in the right position according to 2 abovementioned clinical factors and helps select right dimension of the Healing Abutment to be used as a scaffold while gingival forming.

2. SPECIFICATION


Volume-up™ Gauge




- > Used to guide the position of implant placement and to guide the election of the Healing Abutment dimensions in order to keep the cervical portion of the implant prosthesis at the natural tooth width.
- > Used with the Volume-up™ Parallel Pin for multiple units or bridge.
- > Used with Point Drill (Ø2.1 mm or less).
- > Laser marking identifiable from any position.

※ For the selection of the Healing Abutment, refer the pages 34, 63, 81 & 100.

Volume-up™ Parallel Pin




- > Used for bridge or multiple units with the Volume-up™ Gauge.
- > For bridge or multiple units.
- > For Ø3.5, Ø4.5 and Ø5.5, place the fixture and use the Healing Abutment instead of the Volume-up™ Parallel Pin.




3. PROCEDURE


I. Single Implant




Set the Volume-up™ Gauge on the implant site according to the diameter line marked on the Volume Up™ Gauge.



Position the Point Drill in the drill insertion groove of the Volume-up™ Gauge.



Drill and place the implant in accordance with the manufacturer's implantation sequence.



If implant placement torque is equal to or over 20~30N.cm, connect the Healing Abutment. If not, connect the Cover Screw and do primary closure.

II. Multiple Implants & Bridge



Set the Volume-up™ Gauge and position the Point Drill.



Insert the Volume-up™ Parallel Pin into the hole formed after point drilling.




Carry out the same as the previous step.

* For the selection of the Healing Abutment, refer the pages 34, 63, 81 & 100.


4. CLINICAL CASE




Preoperative view of the healed ridge.



The Volume-up™ Gauge was set to the 8.5 line and point drilling was carried out.



The Ø8.5 Volume-up™ Parallel Pin was inserted into the hole formed by point drilling and point drilling was done at the next site guided by the Volume-up™ Gauge.



The Ø8.5 Healing Abutments were placed after initial & final drilling and fixture placement and bone grafting, and the site was sutured.



After 4 weeks, the contracted buccal alveolar bone & gingiva to the natural shape and width were restored. Which will allow esthetically and functionally great prosthesis fabrication preventing food permeation.

COWELL® REGENERATIVE SOLUTION

Inspire confidence through a comprehensive approach



MegaDerm™ Plus

The acellular dermal matrix can carry out the functional blocks of the membrane due to its long absorption period (soft tissue penetration protection) and is the first in the world with the basement membrane layer removed to maximize the transplant engraftment rate.

COWELL® BMP & INNO GF Kit

The world's first E.rhBMP-2, (E.Coli derived Recombinant Human Bone Morphogenetic Protein type 2), as a growth factor that induces bone and cartilage formation. It is a retinoid mediator that plays a key role in osteoblast differentiation.

INNO-CaP

Osteoconductive synthetic bone graft material consisting of CaP is completely resorpted and progressively replaced by vital bone in the healing period.

DiaDerm® M

Biodegradable atelocollagen membrane is used for GTR & GBR operation. The product, made from high purity atelocollagen, has high biocompatibility, mechanical strength and resistance to enzymatic degradation and flexibility.



INNO OSS & INNO OSS Allo

Allograft composed of 50% of cortical and the other 50% of cancellous. FDBA has been proven out its efficiency and safety by the highest-level pharmacological standards of AATB and is being a global standard of allograft.

InnoGenic® Non-resorbable membranes

The products consisting of Titanium reinforced PTFE membrane (Wifi-Mesh), PTFE membrane (PTFE-Mesh) and Titanium mesh (Ti-Mesh) are non-resorbable membranes to be applied over intraoral defects, especially, tooth extraction and bone augmented sites.

DiaBone

A xenograft is perfectly fused to natural human bone. Diabone has fast blood penetration by giving great hydrophilicity and 3-Dimensional structure which allow optimal cell attachment and blood absorption.

1. Composition of COWELL® BMP

- COWELL® BMP is bone graft material based on the E.rhBMP-2 (E.Coli derived Recombinant Human Bone Morphogenetic Protein type 2), developed for the first time in the world. COWELL® BMP is supported with 10 years of clinical data and over 40 studies.
- BCP/DCP as a carrier allows maintenance of space.

2. Features of COWELL® BMP

- Primary closure for soft tissue regeneration is not required.
- Regenerates adherent gingiva.
- Simplifies challenging bone grafting and soft tissue regeneration.
- Acts directly on stem cells.
- Induces bone regeneration without infection in the extraction socket.
- Contains 1mg of bone morphogenetic protein per 1g of the particle.
(1g of autologous bone contains 2mg of bone morphogenetic protein)

3. Application

A. Orthopedics

Bone grafts

- Fractures: Tibia, Radius, Ulna.
- Spine Fusion (Degenerative Disc Disease):
Interbody cage, Postolateral.

Injection Device

- Lengthening: Distraction osteogenesis.
- Osteoporosis: Hip joint fracture.
- Bone Defect: Bone cyst.
- Bone Fusion: Foot/shoulder revision.

B. Dentistry

Bone grafts

- Severely resorbed alveolar ridges.
- Tooth extraction socket.
- Alveolar bone loss.
- Maxillary sinus bone loss.
- Bone-inductive implant: Coated implant.
- Maxillofacial reconstruction.


C. Dermatology

Soft Tissue grafts


- Damaged skin regeneration.
- Diabetes ulcer.

4. Mechanism of Action of COWELL® BMP

A. Migration of Cells with lamellipodia




B. Cellular mechanisms



- BMP-2 adheres to the membrane of stem cell and induces expression of genes of nucleus. Then, BMP-2 migrates to recipient site.
- BMP-2 growth factor, Twist-2 transcriptional factor, and VEGF growth factor synthesize and secrete endogenous growth factor.
- Proliferation of osteoblast of osteocyte, and proliferation of fibroblast in dermis and keratinocyte of the skin.
- Twist-2 transcriptional factor induces tissue regeneration in osseous tissue and adherent gingival area.

5. Product Type

COWELL® BMP (One vial)



• Dose and particle size of the COWELL® BMP


Product Code	Particle Size
BB1010	0.41~1.0mm

Product Code	Particle Size
BB1025	0.41~1.0mm

Product Code	Particle Size
BB1050	0.41~1.0mm

※ A vial of 0.1g can be used for less than one extraction socket, while 0.25g/0.5g can be used for maxillary sinus or for the wide bone defect area.

COWELL® BMP Plus (Two vials)

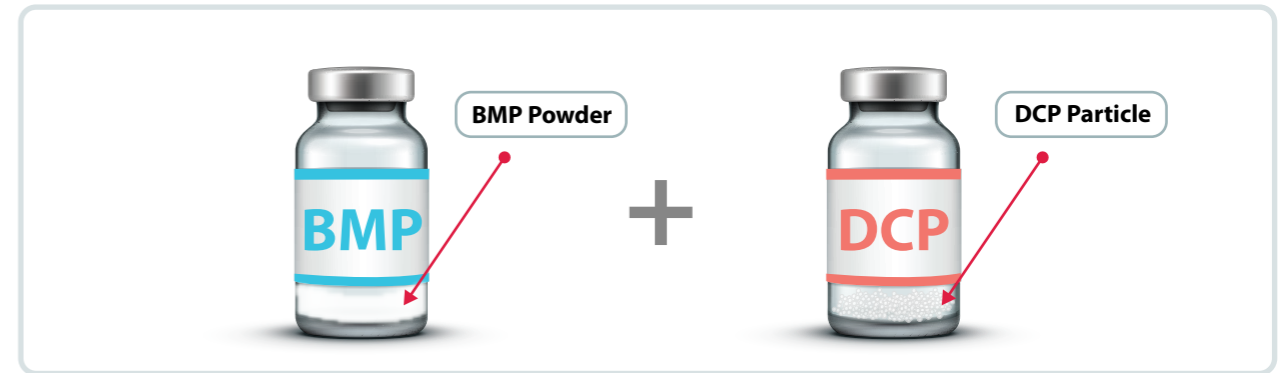

• Dose and particle size of the COWELL® BMP Plus.

BMP 0.1mg

Product Code	BMP Dose	Particle Dose	Particle Size
EBB0125	0.1mg	0.25g	0.41~1.0mm
EBB0105	0.1mg	0.5g	0.41~1.0mm
EBB1100	0.1mg	1g	0.41~1.0mm
EBB1220	0.1mg	2g	0.41~1.0mm

BMP 0.25mg

Product Code	BMP Dose	Particle Dose	Particle Size
EBB2525	0.25mg	0.25g	0.41~1.0mm
EBB2505	0.25mg	0.5g	0.41~1.0mm
EBB1125	0.25mg	1g	0.41~1.0mm
EBB1225	0.25mg	2g	0.41~1.0mm

BMP 0.5mg

Product Code	BMP Dose	Particle Dose	Particle Size
EBB0525	0.5mg	0.25g	0.41~1.0mm
EBB0505	0.5mg	0.5g	0.41~1.0mm
EBB1150	0.5mg	1g	0.41~1.0mm
EBB1250	0.5mg	2g	0.41~1.0mm

BMP 1mg


Product Code	BMP Dose	Particle Dose	Particle Size
EBB1025	1mg	0.25g	0.41~1.0mm
EBB1050	1mg	0.5g	0.41~1.0mm
EBB1011	1mg	1g	0.41~1.0mm
EBB1012	1mg	2g	0.41~1.0mm

BMP 2mg

Product Code	BMP Dose	Particle Dose	Particle Size
EBB2025	2mg	0.25g	0.41~1.0mm
EBB2050	2mg	0.5g	0.41~1.0mm
EBB2011	2mg	1g	0.41~1.0mm
EBB2012	2mg	2g	0.41~1.0mm



INNO GF Kit (Two vials + Saline Solution + Syringe)



• Dose and particle size of the INNO GF Kit.

BMP 0.1mg

Product Code	BMP Dose	Particle Dose	Particle Size
IBB0125	0.1mg	0.25g	0.41~1.0mm
IBB0105	0.1mg	0.5g	0.41~1.0mm
IBB1110	0.1mg	1g	0.41~1.0mm
IBB1220	0.1mg	2g	0.41~1.0mm

BMP 0.25mg

Product Code	BMP Dose	Particle Dose	Particle Size
IBB2525	0.25mg	0.25g	0.41~1.0mm
IBB2505	0.25mg	0.5g	0.41~1.0mm
IBB1125	0.25mg	1g	0.41~1.0mm
IBB1225	0.25mg	2g	0.41~1.0mm

BMP 0.5mg

Product Code	BMP Dose	Particle Dose	Particle Size
IBB0525	0.5mg	0.25g	0.41~1.0mm
IBB0505	0.5mg	0.5g	0.41~1.0mm
IBB1150	0.5mg	1g	0.41~1.0mm
IBB1250	0.5mg	2g	0.41~1.0mm

BMP 1mg

Product Code	BMP Dose	Particle Dose	Particle Size
IBB1025	1mg	0.25g	0.41~1.0mm
IBB1050	1mg	0.5g	0.41~1.0mm
IBB1011	1mg	1g	0.41~1.0mm
IBB1012	1mg	2g	0.41~1.0mm


BMP 2mg

Product Code	BMP Dose	Particle Dose	Particle Size
IBB2025	2mg	0.25g	0.41~1.0mm
IBB2050	2mg	0.5g	0.41~1.0mm
IBB2011	2mg	1g	0.41~1.0mm
IBB2012	2mg	2g	0.41~1.0mm




6. User Guide COWELL® BMP


A. Method I



a. Transfer BCP/DCP graft material (Vial I).



b. Inject distilled water into vial II with lyophilized rhBMP-2 powder in it and mix with the powder.




c. Mix BMP solution with BCP/DCP or plus autogenic / allograft and apply into the recipient site.




d. Cover the defect area using a barrier membrane or suture natural soft tissue without membrane.

B. Method II



a. Transfer BCP/DCP graft material (Vial I) into a container.



b. Apply BCP/DCP into the recipient site and cover the defect area using a barrier membrane or suture natural soft tissue without membrane.




c. Inject distilled water into lyophilized rhBMP-2 powder (vial II).



d. Mix rhBMP-2 with distilled water (saline solution) and wait for 10 to 15 seconds before using.




e. Aspirate the mixture using a syringe.

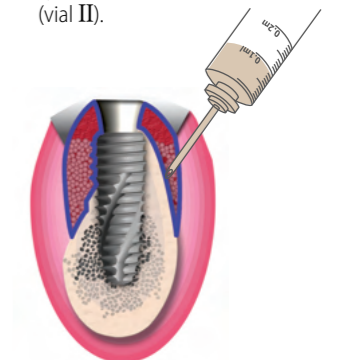


f. Inject BMP solution through soft tissue until needle of syringe reaches bone.

C. Method III




a. Inject distilled water into vial **II** with lyophilized rhBMP-2 powder in it and mix with the powder.

b. Aspirate the mixture using a syringe.



c. Hydrate BMP-2 solution into membrane.




d. Apply BMP-2 solution soaked membrane to damaged site.

Dose of distilled water to make the mixture (BMP-2 Solution)

BMP Dose	Distilled Water Dose	BMP Dose	Distilled Water Dose
0.1mg	0.1ml	2mg	1.6ml
0.25mg	0.2ml	5mg	4ml
0.5mg	0.4ml	10mg	8ml
1mg	0.8ml	20mg	16ml

7. Study Result on COWELL® BMP


In Vivo Study

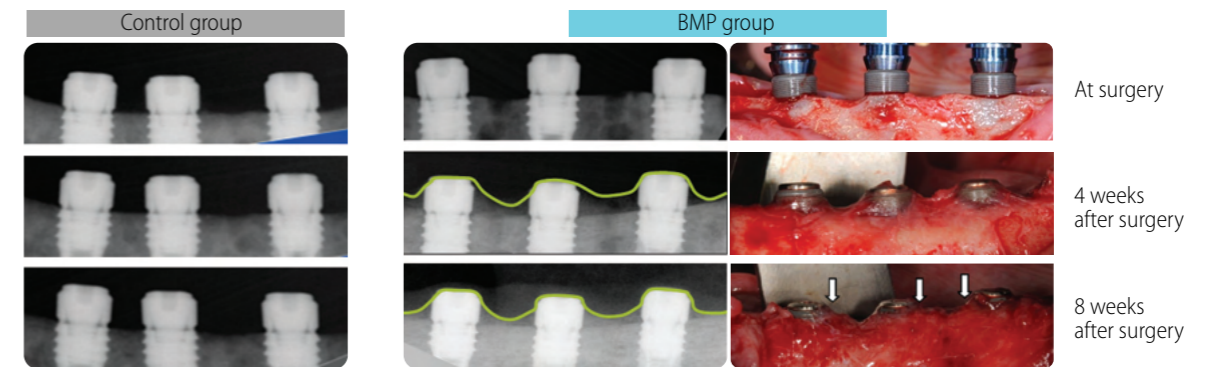

Jung-Bo Huh, et al., Alveolar ridge augmentation using anodized implants coated with Escherichia coli-derived recombinant human bone morphogenetic protein 2 (Beagle dog).

- Oral Surg Oral Med Oral Pathol Oral Radiol Endod 2011.

Histologic Findings: Tissue specimen collected approximately four months after the maxillary sinus grafting (human)



- New bone was formed around the graft material.
- No inflammatory reaction was observed in connective tissue.
- Proliferation of collagen fiber was observed.
- Proliferation of fibrocyte was observed.
- Osteoblast was observed on the surface of newly formed bone.

8. Clinical Data of COWELL® BMP

- Vertical height of surrounding bone was compared three months after grafting in the extraction socket.
- The study was conducted at Seoul National University Bundang Hospital, Yonsei University Dental Hospital, and Korea University Guro Hospital.

Group		Average	SD	95%CI	†P value
Height	Control	-1.087	1.413	(-1.565, -0.609)	0.0006**
	Experiment	-0.059	0.960	(-0.384, 0.266)	
Width at 75% ESL	Control	1.405	1.753	(0.812, 1.998)	0.346
	Experiment	1.863	2.310	(1.081, 2.644)	
Width at 50% ESL	Control	0.542	1.157	(0.15, 0.934)	0.016*
	Experiment	1.239	1.249	(0.816, 1.662)	
Width at 25% ESL	Control	0.006	1.149	(-0.383, 0.395)	<0.0001**
	Experiment	1.279	1.387	(0.81, 1.749)	

ESL: Extraction Socket Level *:P<.05, **:P<.01, †: Student t-test

Jung-Bo Huh, et al., Multicenter, randomized clinical trial on the efficacy and safety of Escherichia-coli-derived rhBMP-2 with β-Tricalcium phosphate and hydroxyapatite in human extraction sockets.

- J Adv Prosthodont 2011;4 -134.

INNO-CaP Calcium Phosphate, Synthetic Bone Graft


Osteoconductive resorbable synthetic bone graft material

- INNO-CaP is an osteoconductive synthetic resorbable bone graft material consisting of Calcium Phosphate.
- INNO-CaP is completely resorpted and progressively replaced by normal-structured bone in the healing period.

Excellent Biocompatibility and Conductivity

- The characteristic biocompatibility and conductivity of the INNO-CaP represent the most safety.


Cell culture SEM images (14 days)



A porosity for new bone ingrowth

- The porosity promotes ingrowth of osteoblast, osteoclast and growth factors.

Particle surface SEM image



Indications

Sinus graft surgery

- For sinus graft, INNO-CaP is used alone or in combination with the other graft materials.
- Various healing period according to residual bone height.

residual bone height	less than 1mm	2~4mm	more than 4 mm
implant placement	post operation 9~12 months	post operation 6 months	simultaneous placement

GBR (Guided Bone Regeneration)

- Minimize the amount of autogenous bone.
- Sub-graft materials.
- Vertical and lateral augmentation.
- Using with the COWELL® BMP is highly recommended.

Dose and Particle Size

Product Code	Particle Size	Particle Dose
IG1025	0.4~1.0mm	0.25g
IG1050		0.5g
IG1001		1g
IG1002		2g
IG1425	1.0~1.4mm	0.25g
IG1450		0.5g
IG1401		1g
IG1402		2g



INNO OSS & INNO OSS Allo

Allograft


FDBA, Cortical 50% Cancellous 50%

Product Features

- This product is made up of human tissue from trusted donors whose gender, age, and medical history were checked to ensure that their tissue could be used safely.
- It is an ideal combination of 50% cortical powder and 50% cancellous powder for bone induction.
- The 50% cortical powder maintains the space of the transplanted area during the new bone formation due to the delayed absorption rate. [OsteoConduction]
- 50% cancellous powder is rich in minerals and collagen that promote cell adhesion, bone remodeling, and vascular re-formation. [OsteoInduction]
- To prevent cross-infection by a different donor, the process is done by a single donor.
- Under the higher-level pharmacological standards (medical criteria) of the American Association of Tissue Banks (AATB), we sampled, processed and distributed the allograft tissue.
- We recommend use of this product with the COWELL® BMP.
- The difference between INNO OSS and INNO OSS Allo is classification of the product only. INNO OSS is classified as a HUMAN TISSUE and INNO OSS Allo is a MEDICAL DEVICE.




SEM Image



Dose and Particle Size

Type	Product Code	Particle Size	Partide Dose
INNO OSS	OSS3	0.3~0.8mm	0.3cc
	OSS6	0.3~0.8mm	0.6cc
INNO OSS Allo	OSS3P	0.3~0.8mm	0.3cc
	OSS6P	0.3~0.8mm	0.6cc

Method of Use




DiaBONE

Bovine Bone Substitute


A Bone 100% fused to Natural Human Bone

- Fast blood penetration.
- Great hydrophilicity.
- 3-Dimensional structure.
- Easy to handle.
- Maximizes bone fusion.
- Mutually connected porous structure.
- Optimal cell attachment and blood absorption.
- Stimulates activity of osteoclast and osteoblast.



Safe & Trustable Material

- Made of 100% bovine bone.
- Cleansing over 30 times to perfectly remove organic substances.
- Firmed bone formation as highly dense.
- 100% pure HA & 99.73% of bone crystallization.



(New bone formation clearly observed around grafted bone site)

Volume and Particle Size

Product Code	Partide Size	Volume
G2015	0.25~1.0mm	0.15g
G2025	0.25~1.0mm	0.25g
G2050	0.25~1.0mm	0.5g
G2100	0.25~1.0mm	1g
G2200	0.25~1.0mm	2g

Product Code	Partide Size	Volume
G5015	1.0~2.0mm	0.15g
G5025	1.0~2.0mm	0.25g
G5050	1.0~2.0mm	0.5g
G5100	1.0~2.0mm	1g
G5200	1.0~2.0mm	2g


MEGA DERM™ PLUS Acellular Dermal Matrix

Product Features


- This product can carry out the functional blocks of the membrane (soft tissue penetration protection) due to its long absorption period, and has excellent manipulability.
- This product is produced under the stringent standards of the MFDS.
- The world's first E-Beam sterilization can induce safe and prompt engraftment.
- E-Beam is safe and can be effectively sterilized without destroying the collagen tissue structure.
- This product is the first in the world with the basement membrane layer removed (patent pending) to maximize the transplant engraftment rate.
- This shows the high engraftment rate after the transplant by maximizing the influx of fibroblasts and/or the neovascularization. (Patent Application No. 10-2012-0026616)



MEGA DERM PLUS three-dimensional structure of the dermis




The world's first 'E-Beam' sterilization that does not destroy the collagen structure



Application

- Mucogingival defect.
- Soft tissue formation around the implant area.
- Wide perforation in the Schneiderian membrane.

SEM Images (They have kept the collagen structure after the E-Beam sterilization.)



A. SEM (x200) B. SEM (x20,000) C. TEM (Transverse section) D. TEM (Cross section)

Specifications

Product Code	Size	Thickness
D1520P	15x20mm	0.5~0.7mm
D1525P	15x25mm	0.5~0.7mm

Diaderm® M Biodegradable Atelocollagen Membrane

GTR(Guided Tissue Regeneration) GBR(Guided Bone Regeneration) membrane

- Diaderm® is a dental membrane used for GTR (Guided Tissue Regeneration) and GBR (Guided Bone Regeneration) operation.
- Diaderm® helps restoration of alveolar bone and protect operation site from infiltration of an epithelial cell and exterior circumstances.
- Diaderm® made from high purity atelocollagen has high biocompatibility, mechanical strength, resistance to enzymatic degradation and flexibility.


Product Features

- High biocompatibility.
- Induces restoration of tissue.
- Closes wound site completely.
- Sustains space for bone reproduction.
- Easy to handle and operate.



Resistance against enzymatic degradation

- Diaderm® has higher resistance to enzymatic-degradation compared to products from other manufacturers.



Storage and Shelf Life

- Store at 1-30°C
- Shelf Life : 3 years from the date of manufacture

Specifications

Product Code	Size
AS-007020	15X30mm


InnoGenic® Non-resorbable Membrane

InnoGenic® Wifi-Mesh and InnoGenic® PTFE-Mesh


- The InnoGenic® Wifi-Mesh, PTFE-Mesh and Ti-Mesh are non-resorbable barrier membranes to be applied over intraoral defects, especially, tooth extraction and bone augmented sites. The InnoGenic® Wifi-Mesh and PTFE-Mesh are made of proprietary 100% PTFE, the polytetrafluoroethylene (teflon) sheet which is a biologically inactive and tissue compatible material and the InnoGenic® Wifi-Mesh is reinforced with titanium frames (Titanium Gr II, ASTM F 67) embedded between two layers of PTFE sheets.

InnoGenic® Wifi-Mesh


> Packing unit: 1ea



Product Code	Size	Thickness
BTP1424AA	14X24	0.25
BTP1424AB	14X24	0.25
BTP1525BB	15X25	0.25
BTP1725CA	17X25	0.25
BTP2030AB	20X30	0.25
BTP2530AB	25X30	0.25
BTP3040AB	30X40	0.25




Clinical Case using the Wifi-Mesh

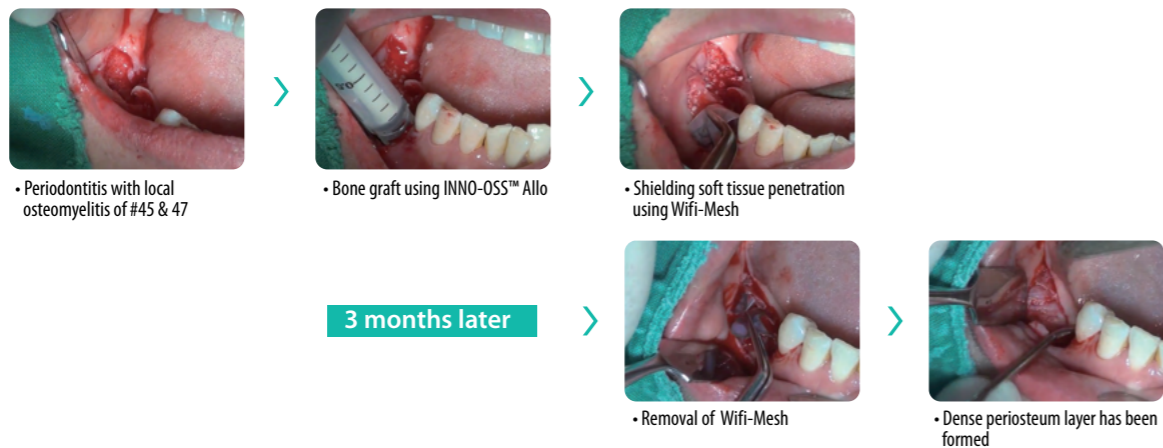

InnoGenic® PTFE-Mesh

> Packing unit: 5ea



Product Code	Size	Thickness
TS17251	17 x 25	0.1
TS24301	24 x 30	0.1
TS17252	17 x 25	0.2
TS24302	24 x 30	0.2

Features

- **Non-resorbable:** Made of 100% non-resorbable material for users to modulate healing period.
- **Non-porous (0.0 μm) + Open Membrane Sheet Technique:** Prevention of infection or other possible defects caused from passage or integration of bacteria through porosity of plaster and it even allows to apply Open Membrane Sheet Technique.
- **Prevention of Displacement:** Not only being sutured along with gingiva but also being fixed with components from the InnoGenic® GBR Kit to prevent displacement of the product.
- **Close to Transparency:** Observation of the healing of the underlying tissue through almost transparent PTFE surface allows more predictable result and helps determine removal time easier.
- **Easy to be Customized:** Easy to modify the shape according to shape and dimension of the defect.
- **Easy to be Removed :** Put a hook in the hole of the titanium frame of the InnoGenic® Wifi-Mesh and in any center part of the InnoGenic® PTFE-Mesh and remove.

Comparison to other similar products sold in market

Classification	Product A	Product B	InnoGenic® Wifi-Mesh & PTFE-Mesh
SEM Photograph			
Ultrastructure	Fiber	Filter	Sheet
Bacterial infection at exposure	Bacterial toxin penetration between filters at 50 μm intervals	Bacterial toxin penetration between filters at 2 μm intervals	No Bacterial toxin penetration thanks to non porous structure
Action on Exposure	Instant Removal	Removal on week 3 to 4	Safe for more than 6 weeks
Shielding Function against Fiber Cell	High	High	Extremely High
Shape-keeping Capability against External Force	Large Deformation	Shrinkable Deformation	No Deformation

InnoGenic® Ti-Mesh

- The InnoGenic® Ti-Mesh is made of stamping titanium sheet, also Titanium Gr II, ASTM F 67, which is 100% commercially pure titanium. The InnoGenic® Ti-Mesh is non-resorbable surgical mesh to be applied over intraoral defects, especially, tooth extraction and bone augmented sites.



Product Code	Size	Thickness
TMP210	25 x 34	0.07
TMP211	25 x 34	0.1

Features

- **Easy to be Customized:** Easy to modify the shape according to shape and dimension of the defect.
- **Prevention of Displacement:** Prevents displacement of the InnoGenic® Ti-Mesh using the InnoGenic® GBR Kit inserted and fixed into the 1mm hole of the Ti-Mesh Frame.
- **No Memory:** The problem of Majority of Titanium Meshes in the market is resilience of the products after certain time. Due to this problem, patients go through serious pain. The InnoGenic® Ti-Mesh is, however, made after many times of stamping process, the InnoGenic® Ti-Mesh does not come back to the original shape after shape is formed.

Ver.29
Help your daily practice superior



CWM-Ver.29

Cowellmedi Co.,Ltd

Floor 6, Blue Fin Tower, 42, Seochojungang-ro, Seocho-gu, Seoul, Korea
Tel. +82-2-3453-5085 Fax. +82-2-3453-5086 E-mail. cib@cowellmedi.com

Cowellmedi USA INC

218 Trianon LN Villanova PA 19085-1442 USA
Tel. 1-623-939-1344 Fax. 1-623-939-1472

Cowell R&D Institute

48, Hakgam-daero 221beon-gil, Sasang-gu, Busan, 46986, Korea
Tel. +82-51-314-2028 Fax. +82-51-314-2026



Cowellmedi Co., Ltd. www.cowellmedi.com